

1/36

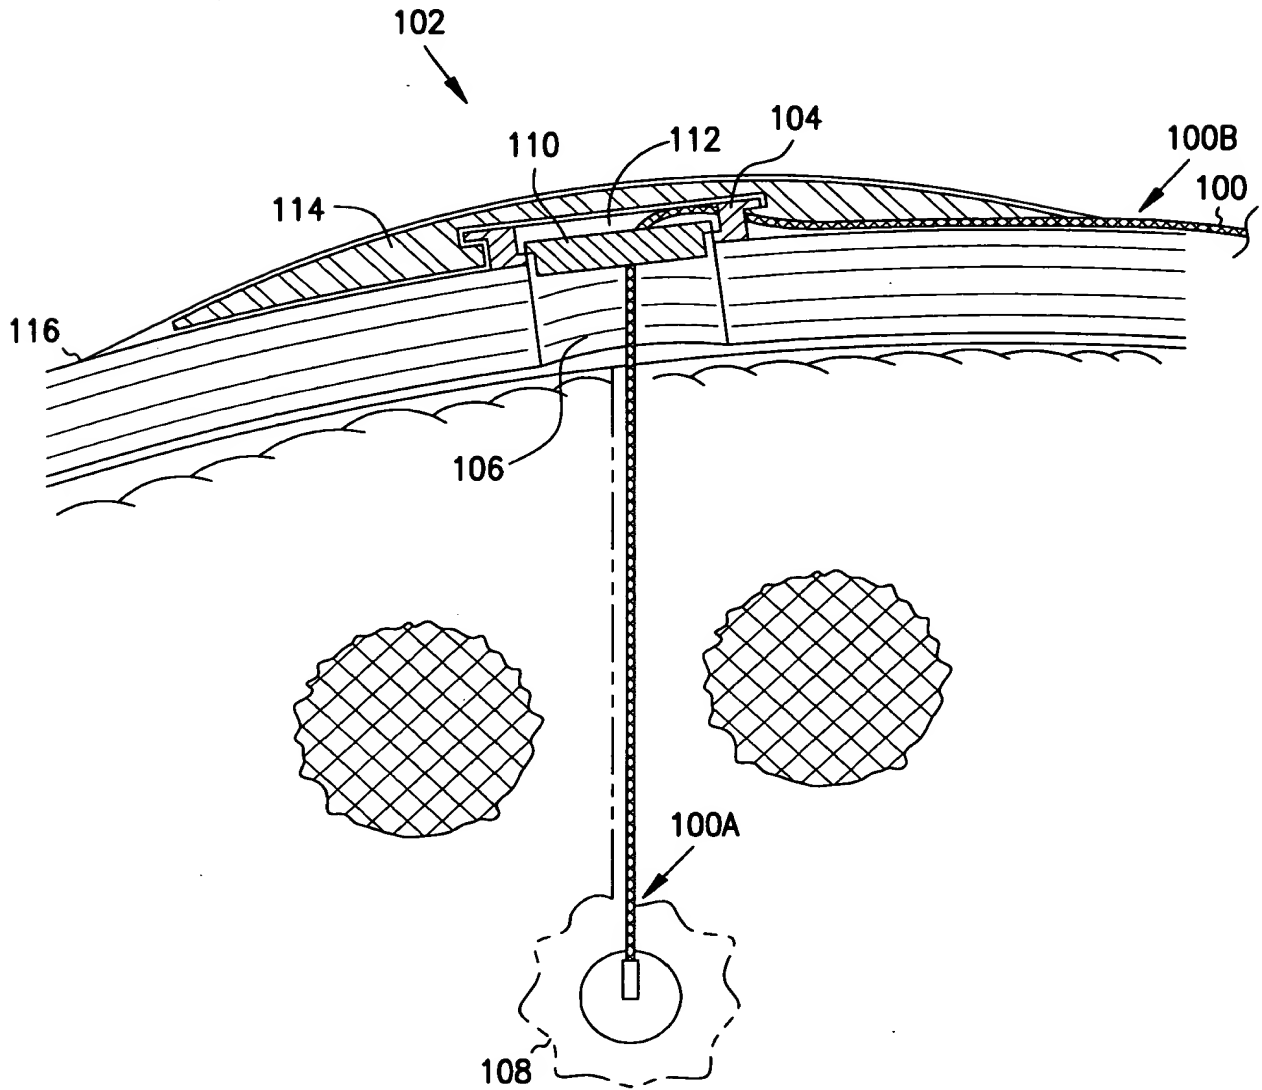


FIG. 1

2/36

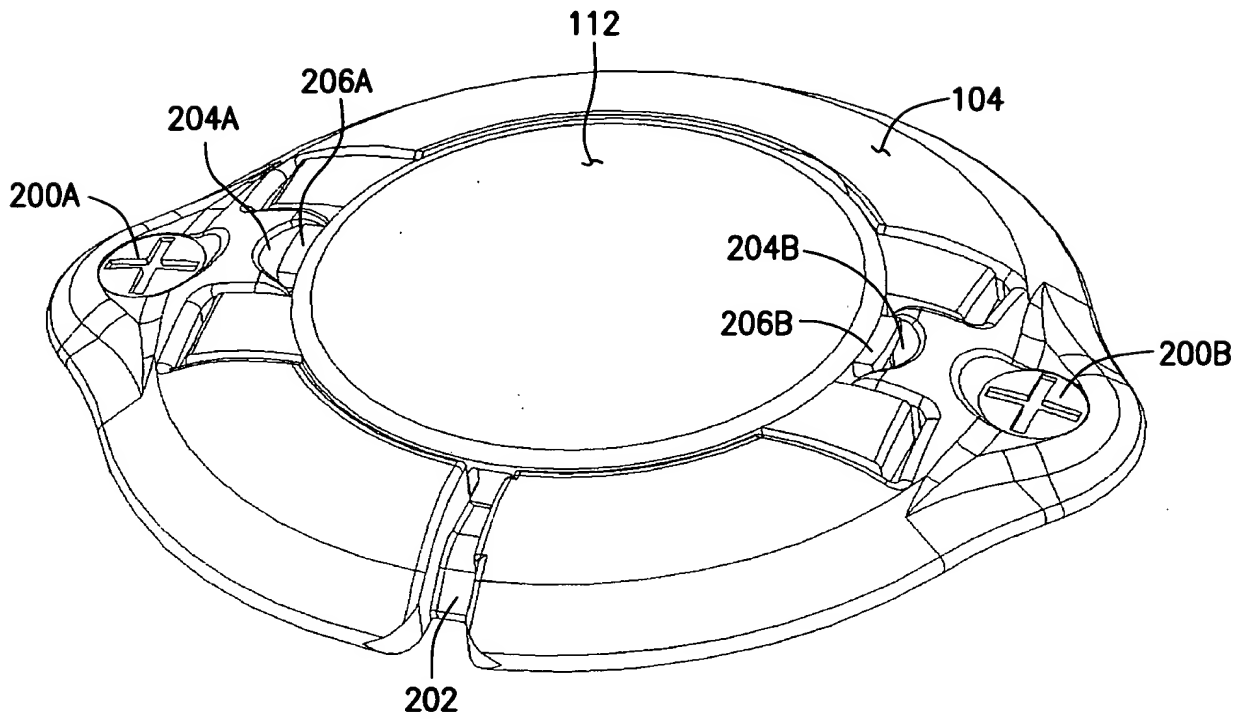


FIG. 2

09/828,451 0828451

3/36

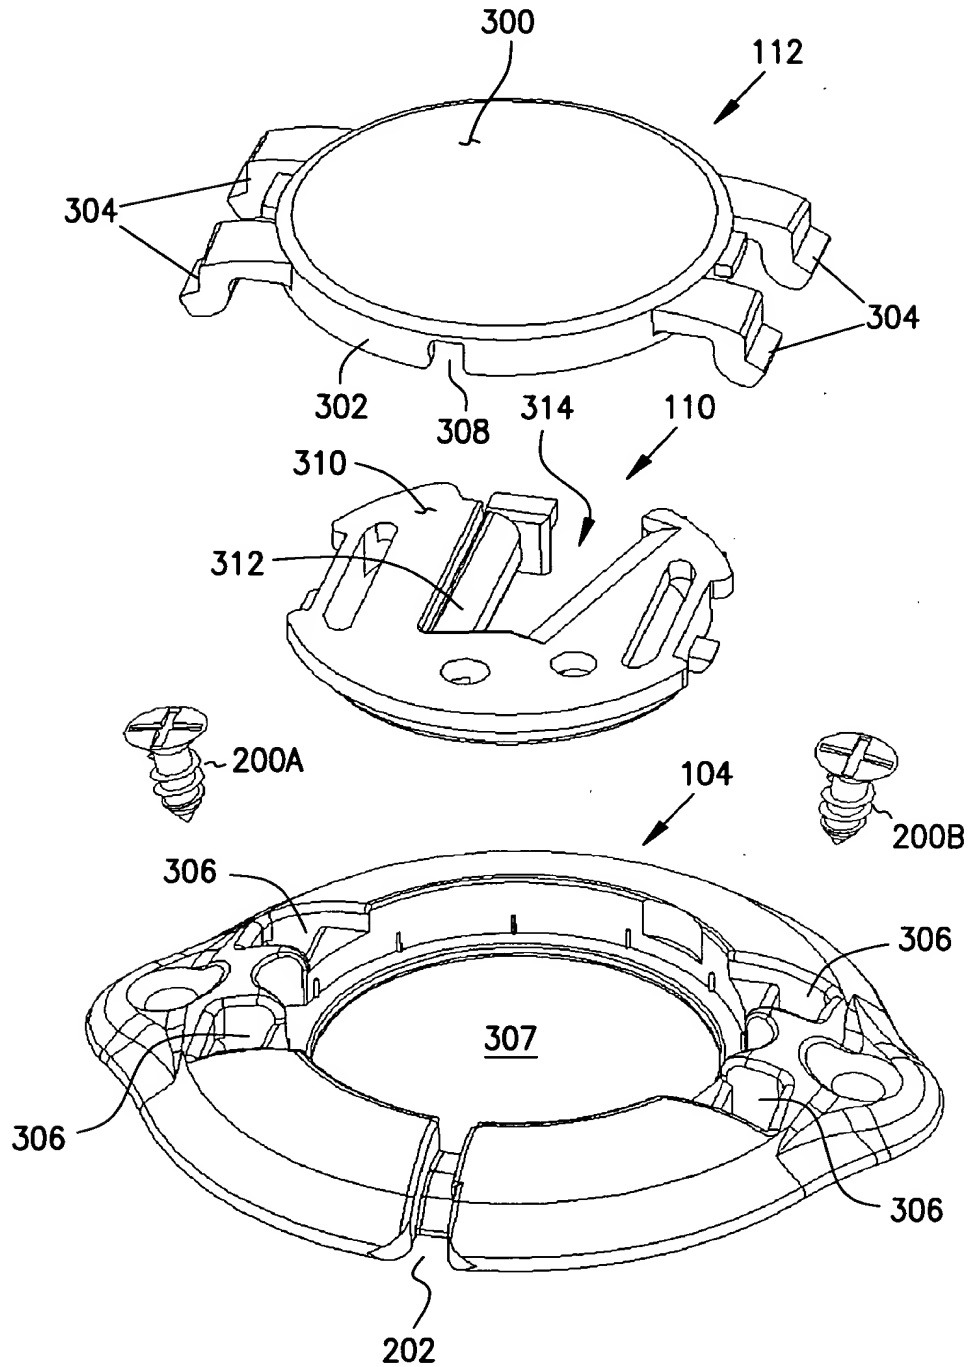


FIG. 3

09/828,451-0800 T 09/828,451

4/36

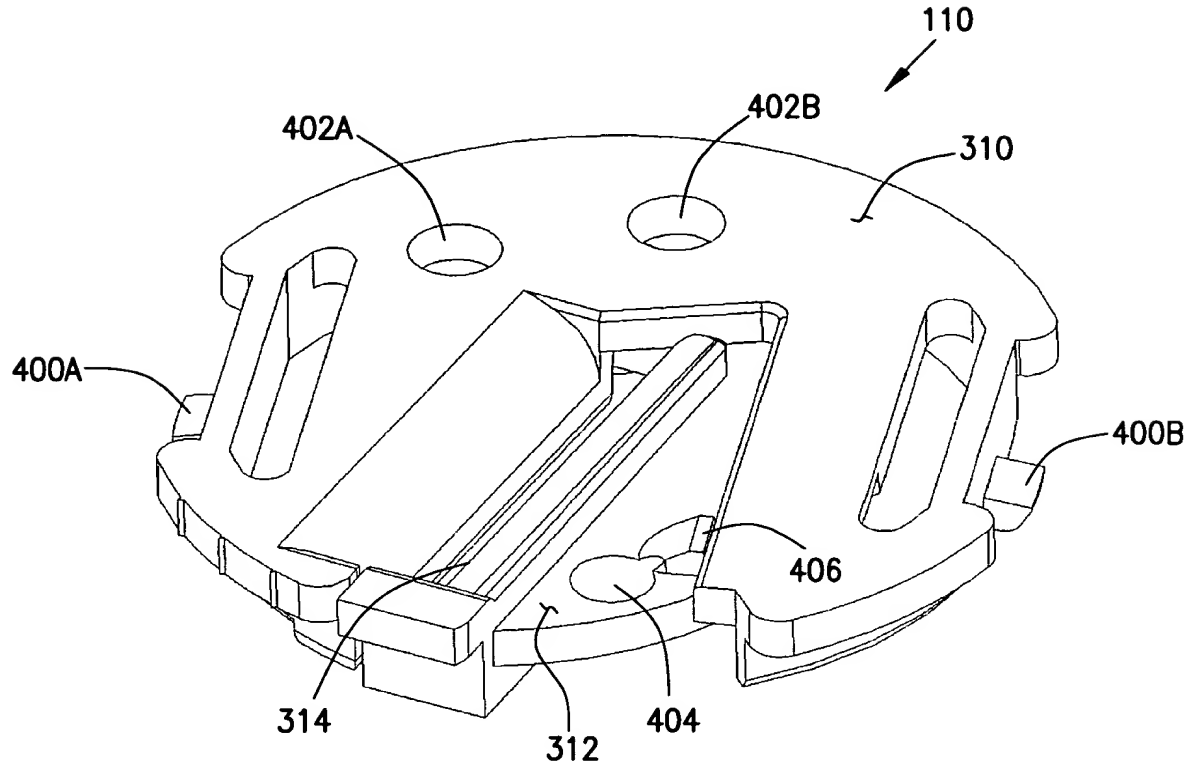


FIG. 4

09828451 038660

5/36

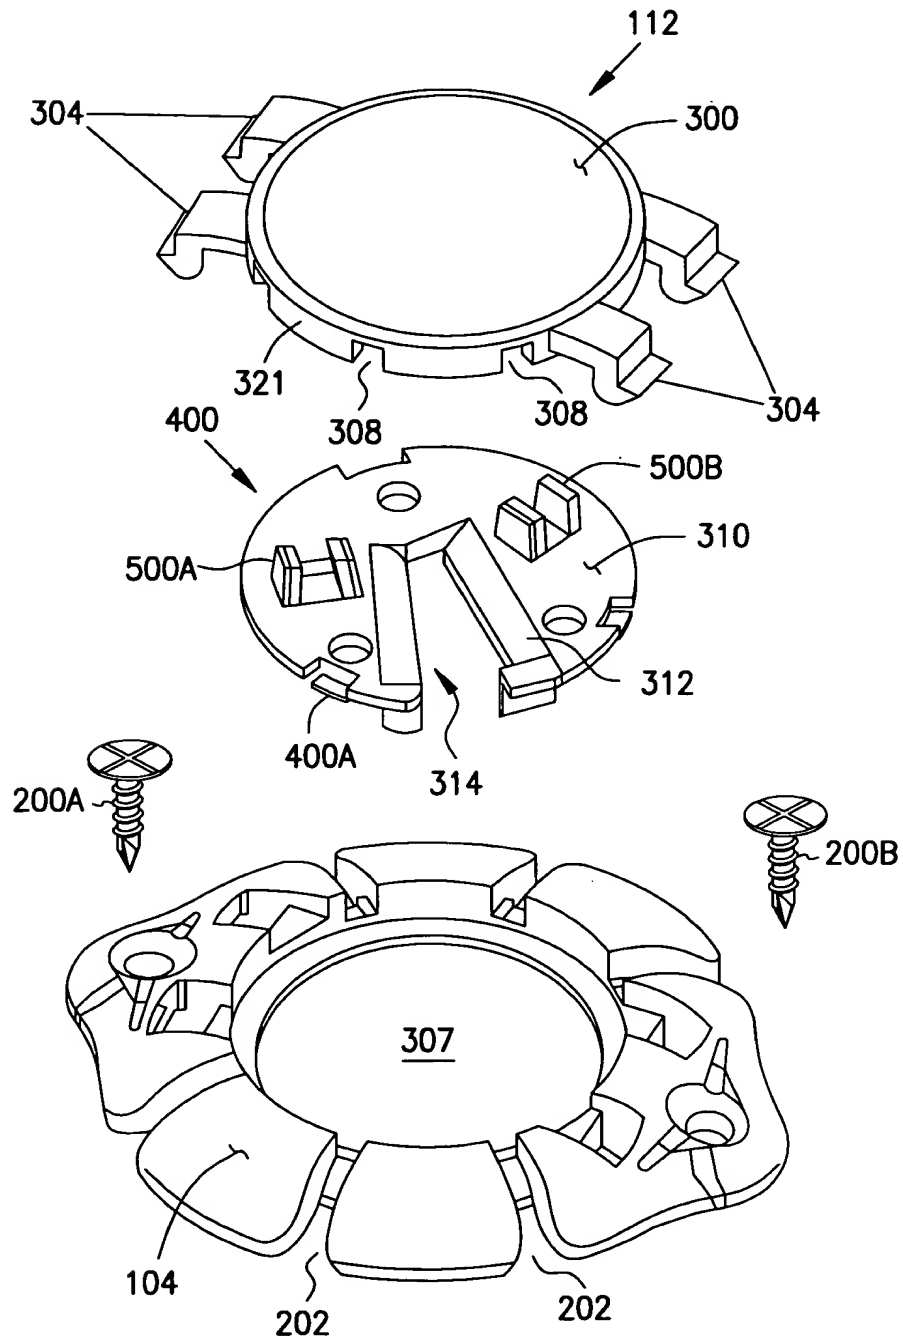


FIG. 5

6/36

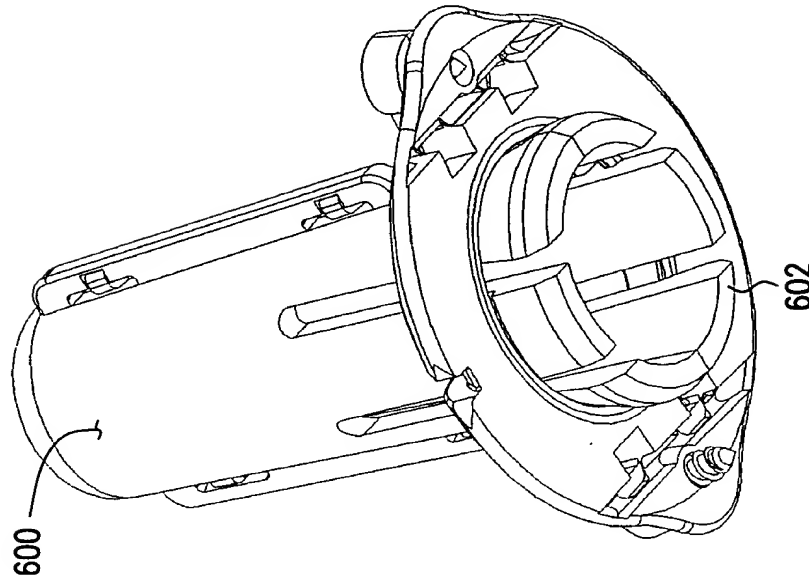


FIG. 6B

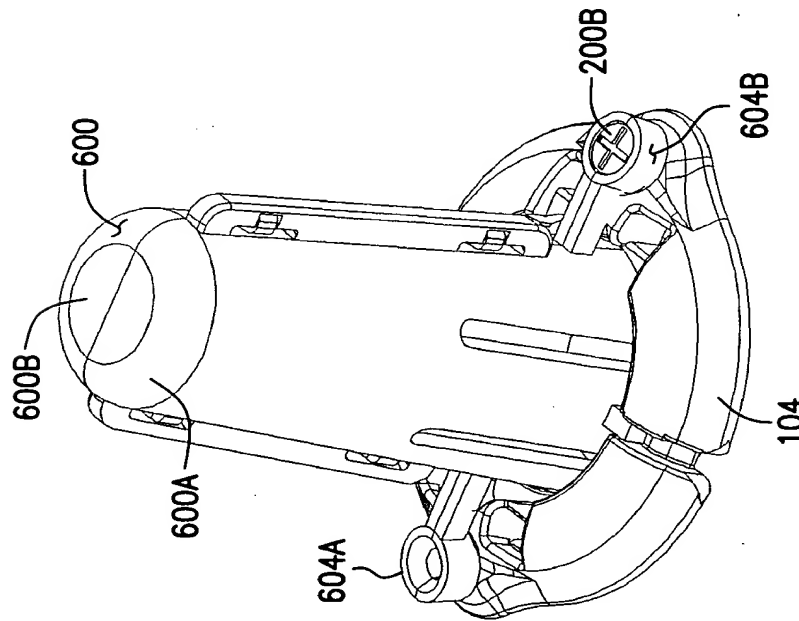


FIG. 6A

100280" 09/82860

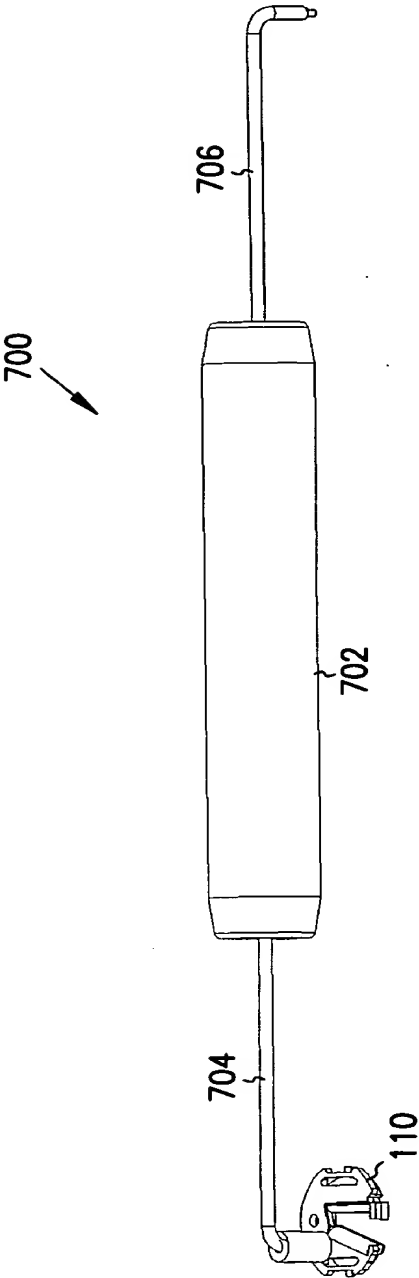


FIG. 7

8/36

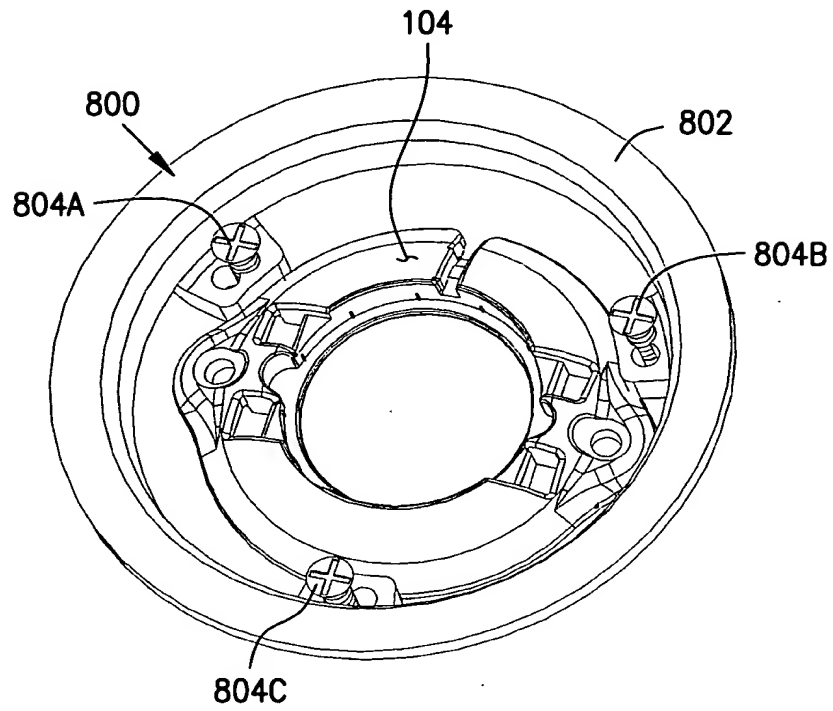


FIG. 8

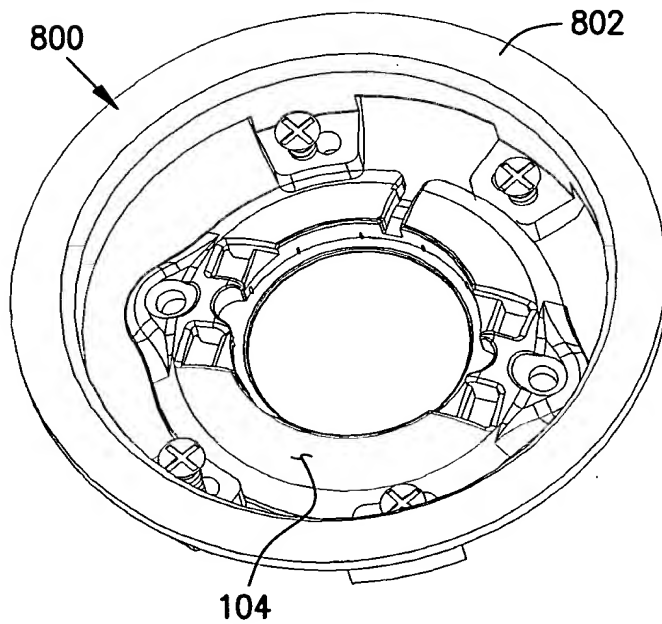


FIG. 9

1002280" 1542360



9/36

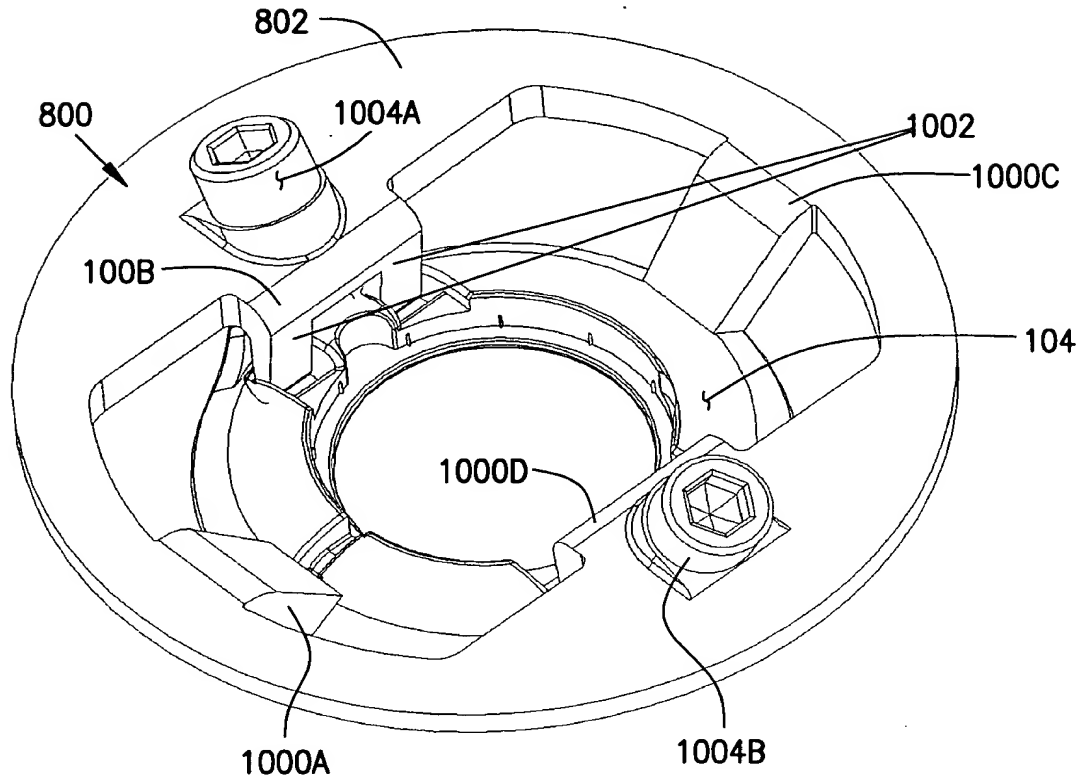


FIG. 10

09828451.082860

10/36

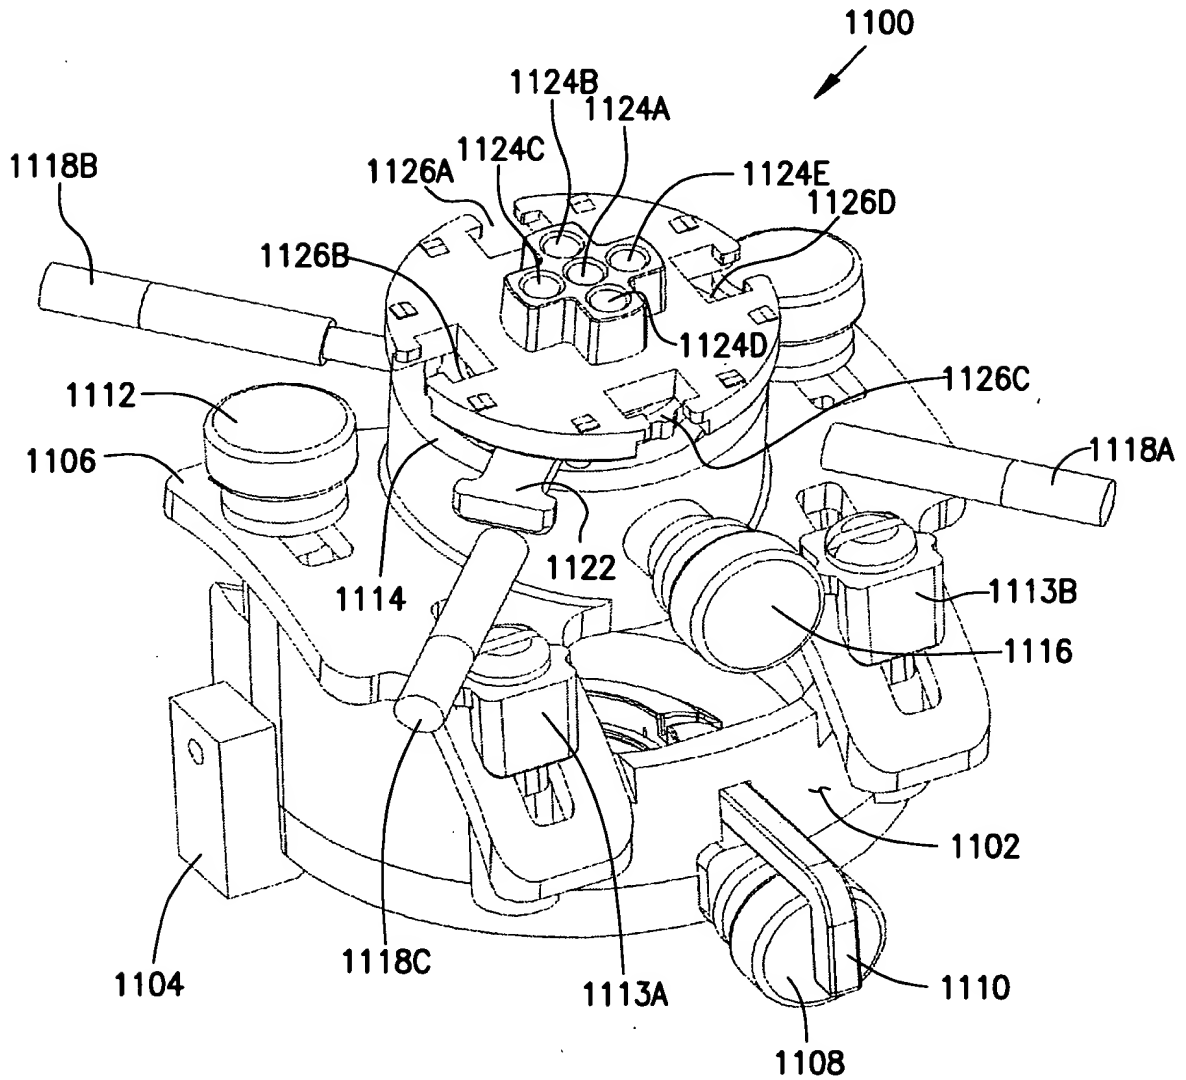


FIG. 11

09828451 "082001

11/36

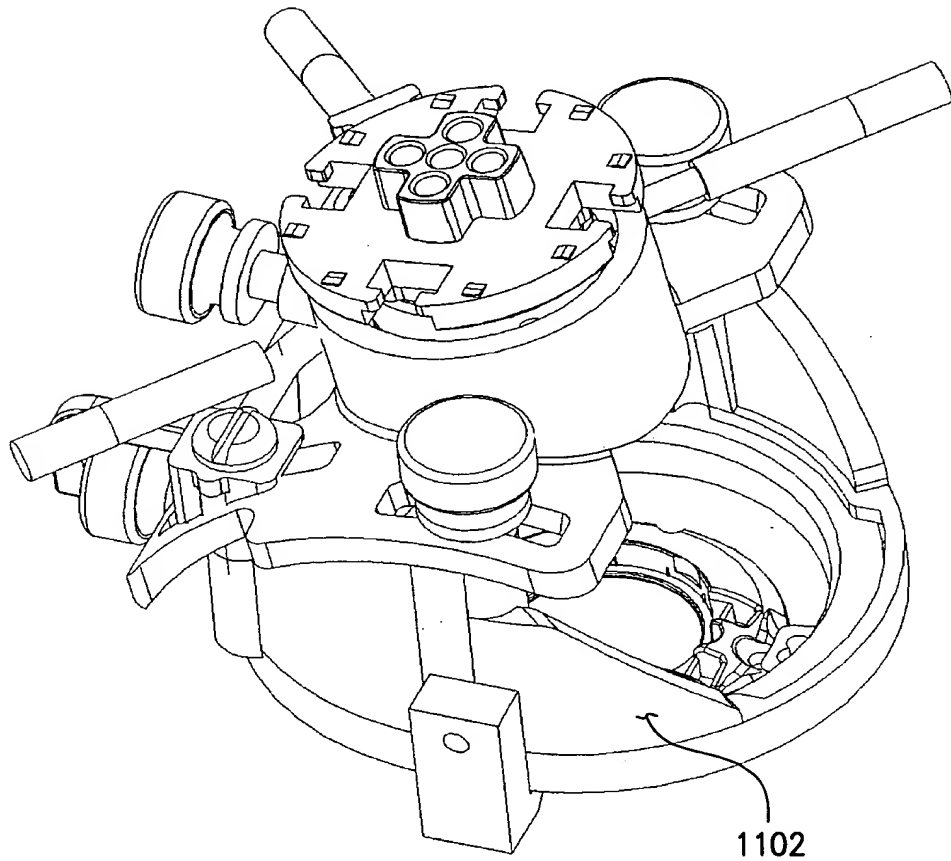


FIG. 12

12/36

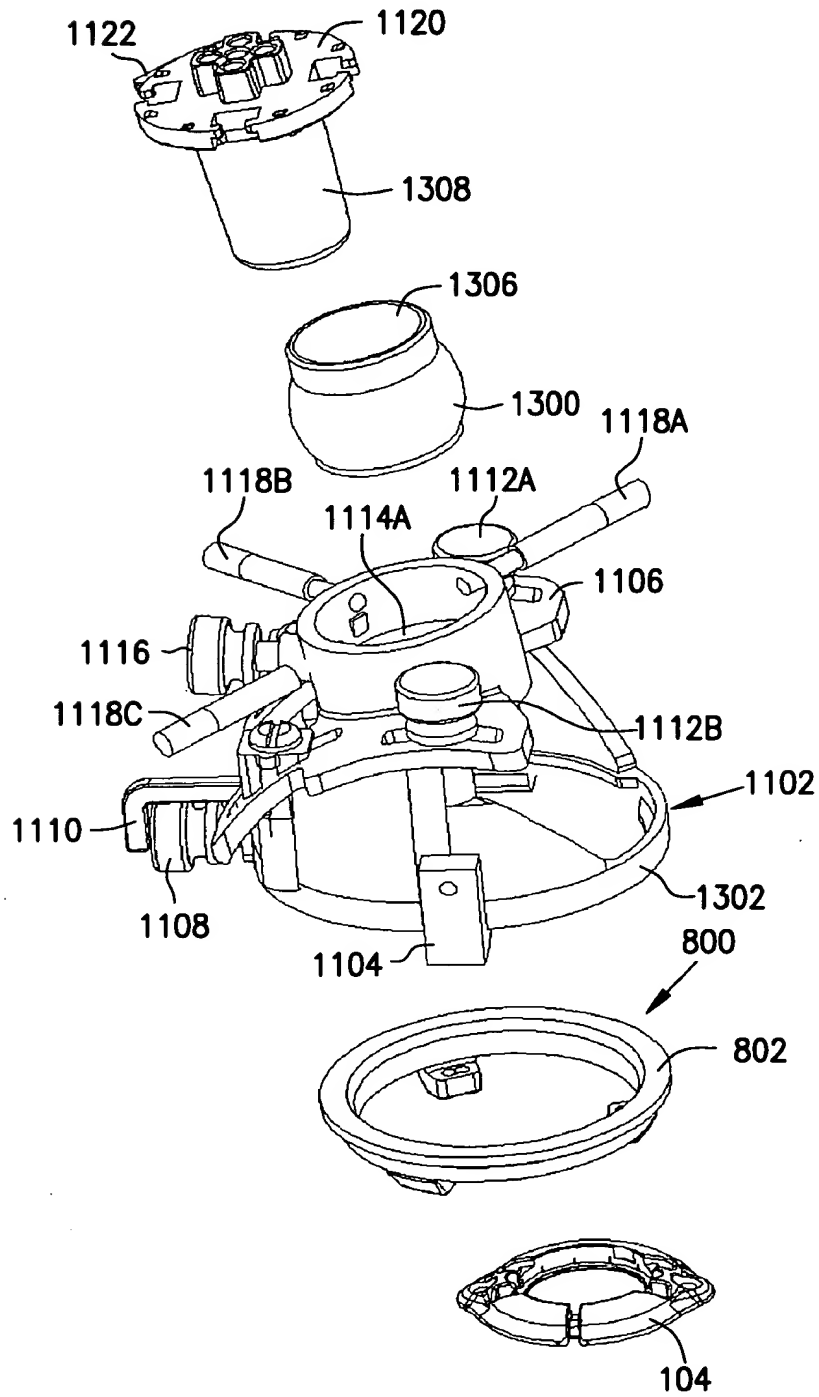


FIG. 13

09/828,451-0001

13/36

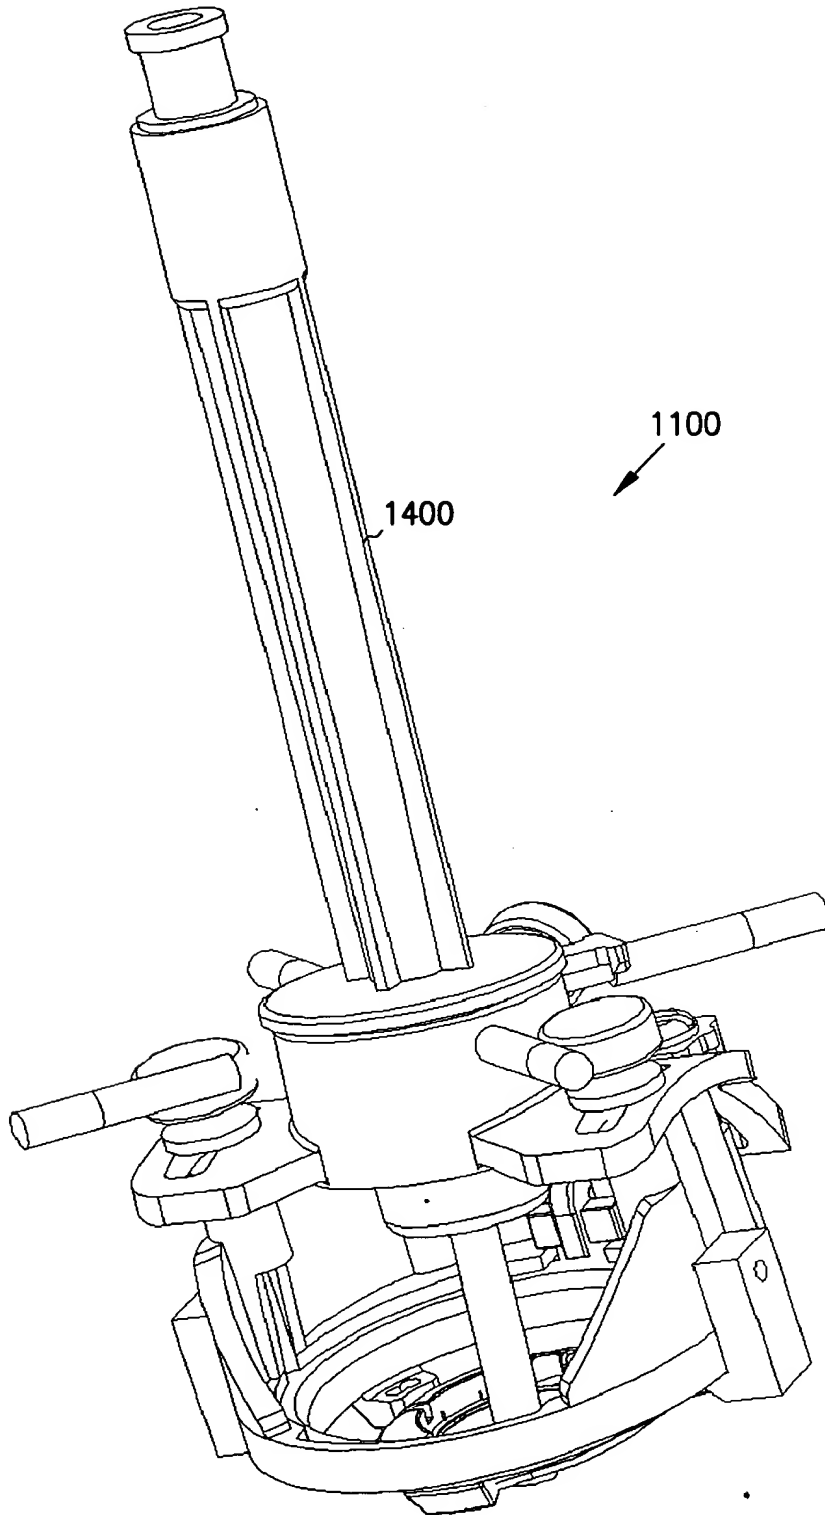


FIG. 14

09828451.082001

14/36

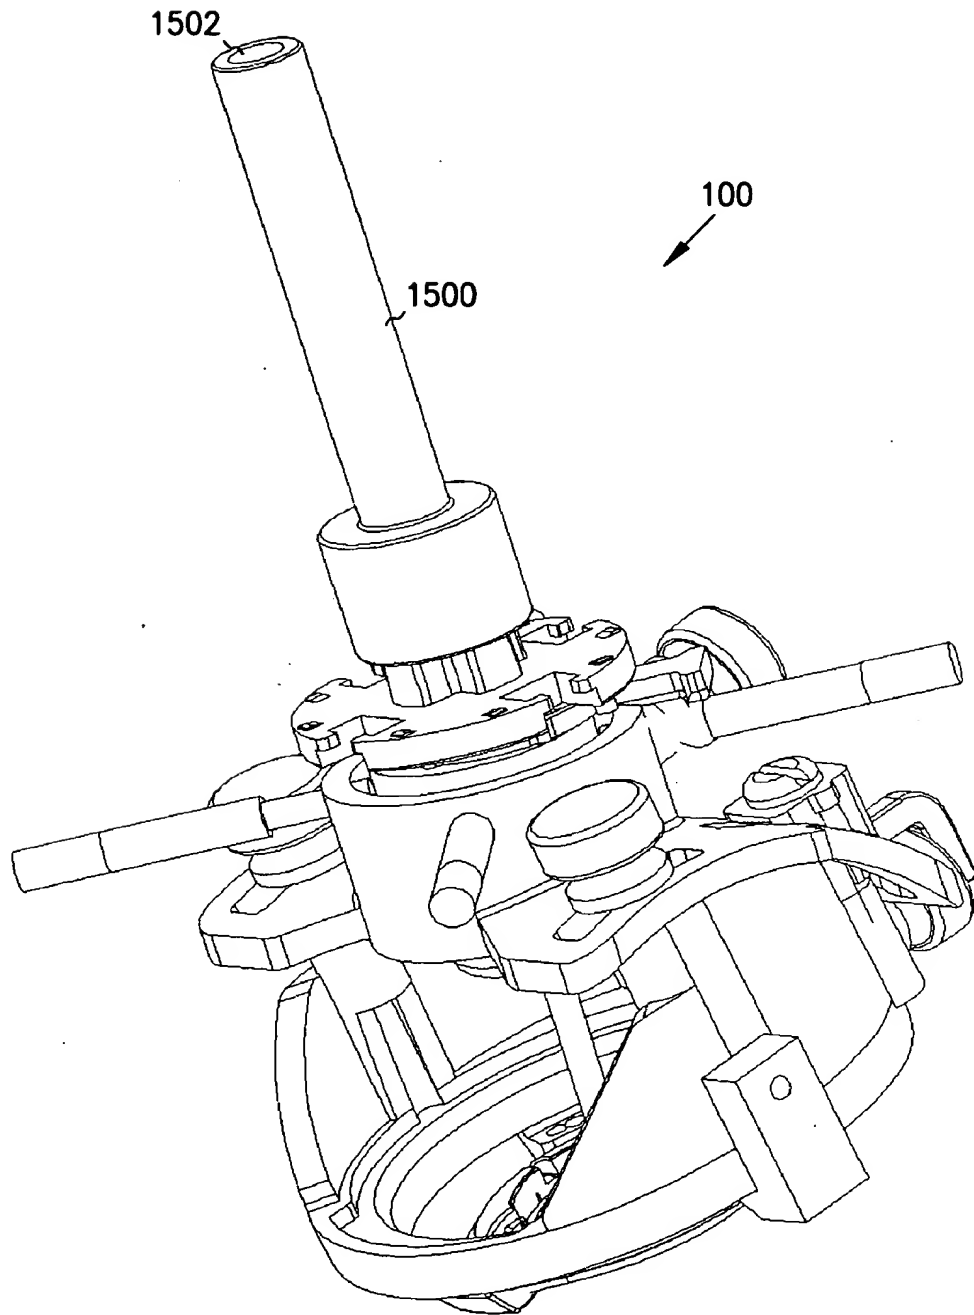


FIG. 15

09828451 082001

15/36

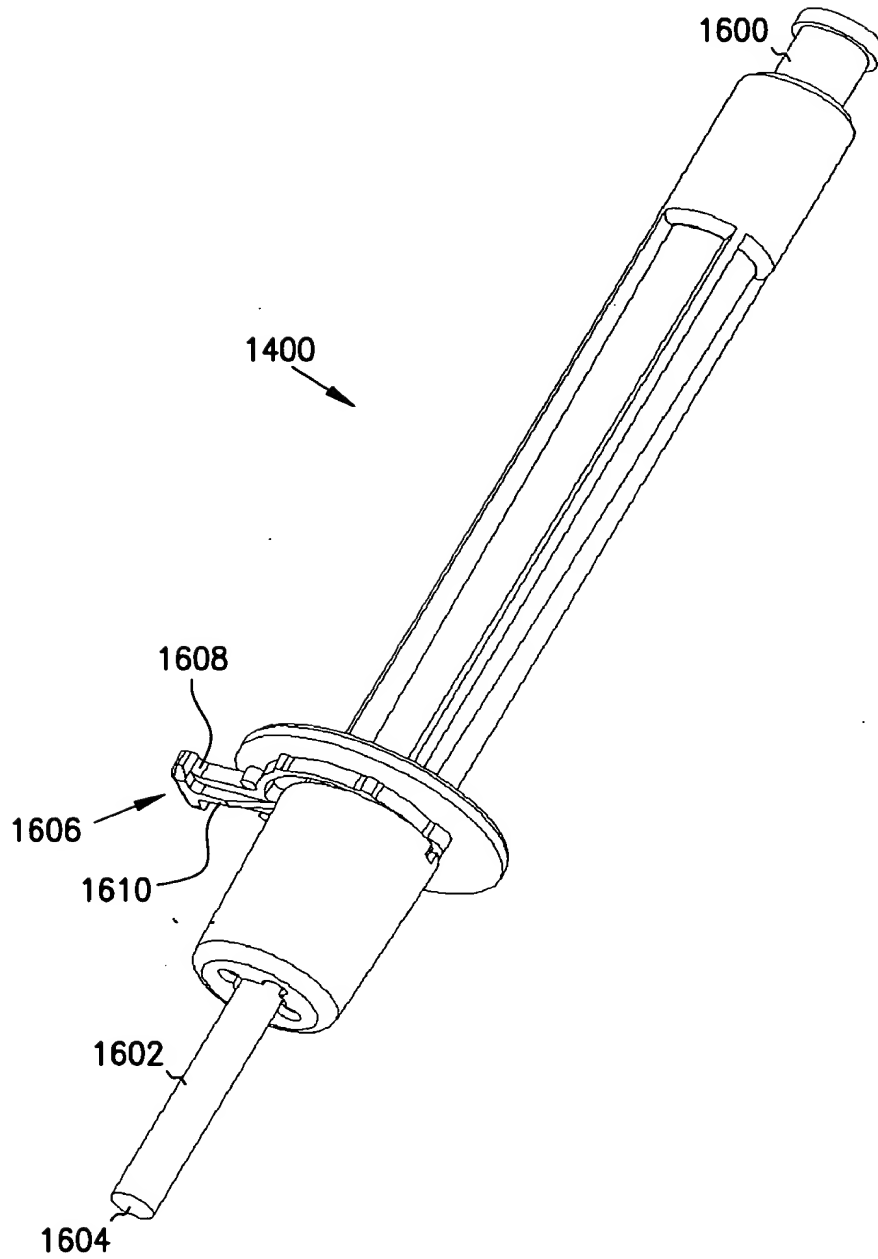


FIG. 16

09828451 082004

16/36

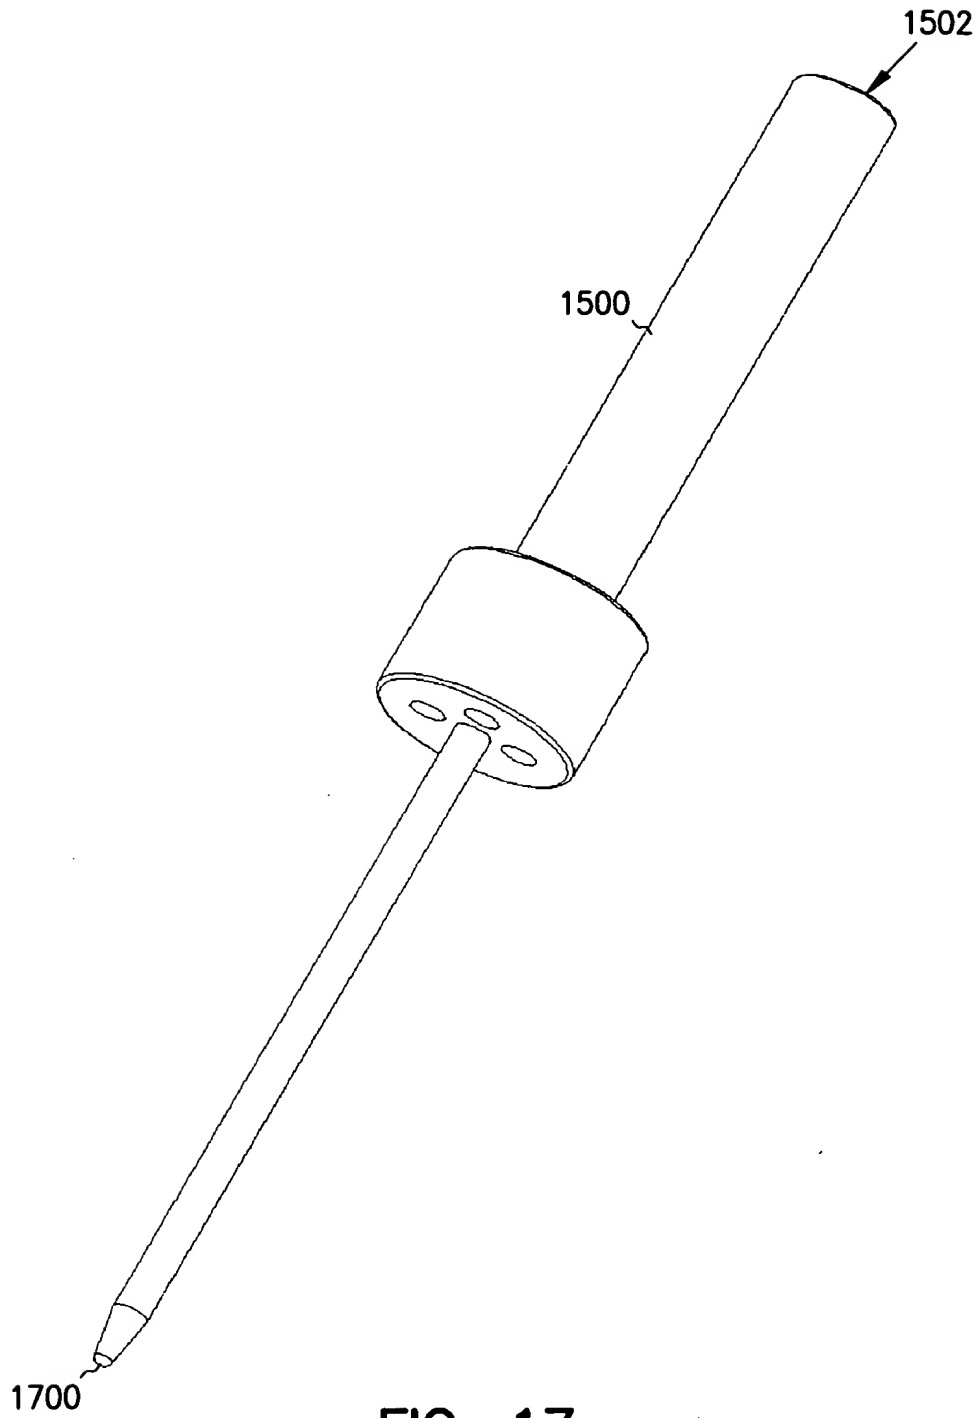


FIG. 17

09/828,451 F5432850



17/36

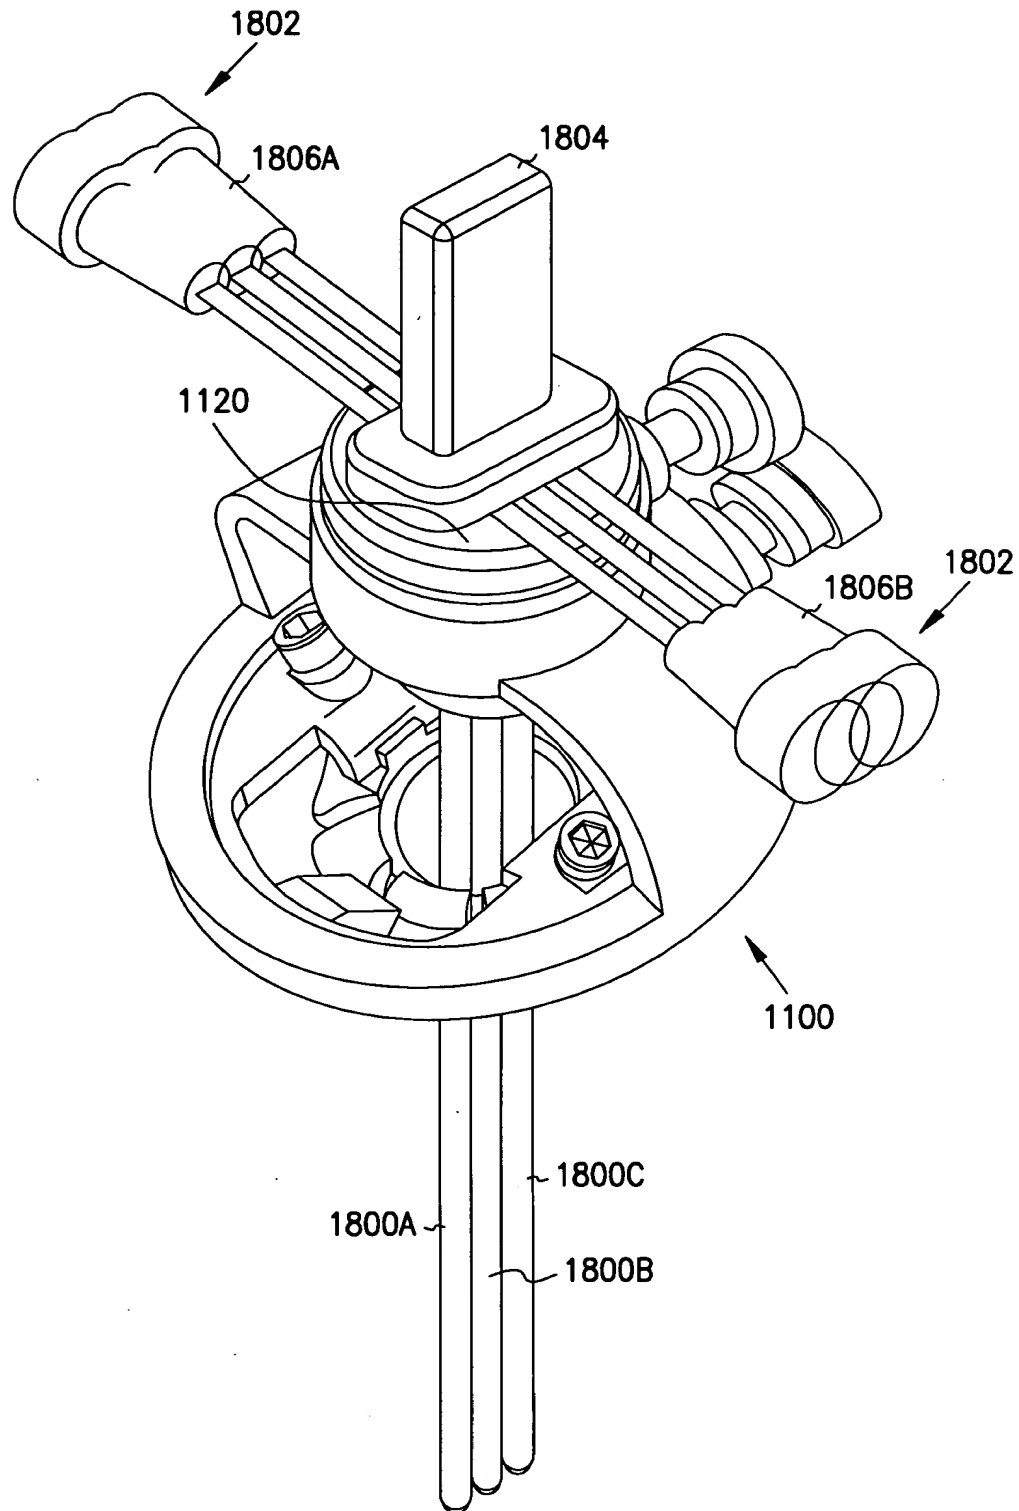


FIG. 18

09/828,451

18/36

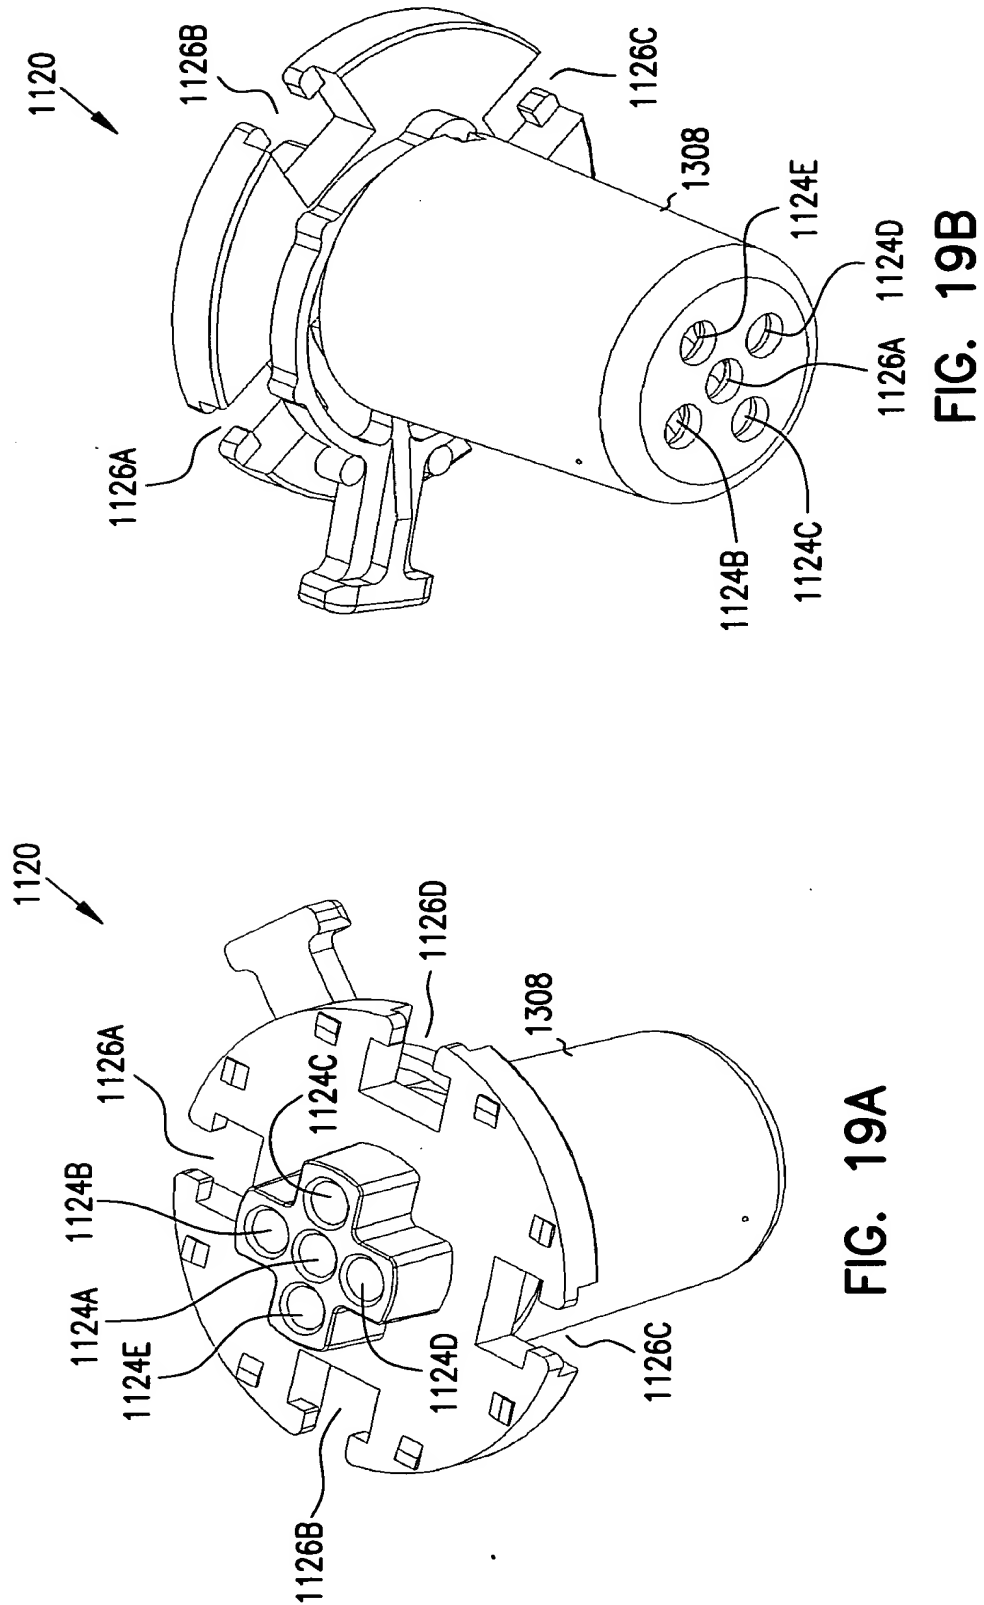


FIG. 19A

FIG. 19B

FIG. 19A

19/36

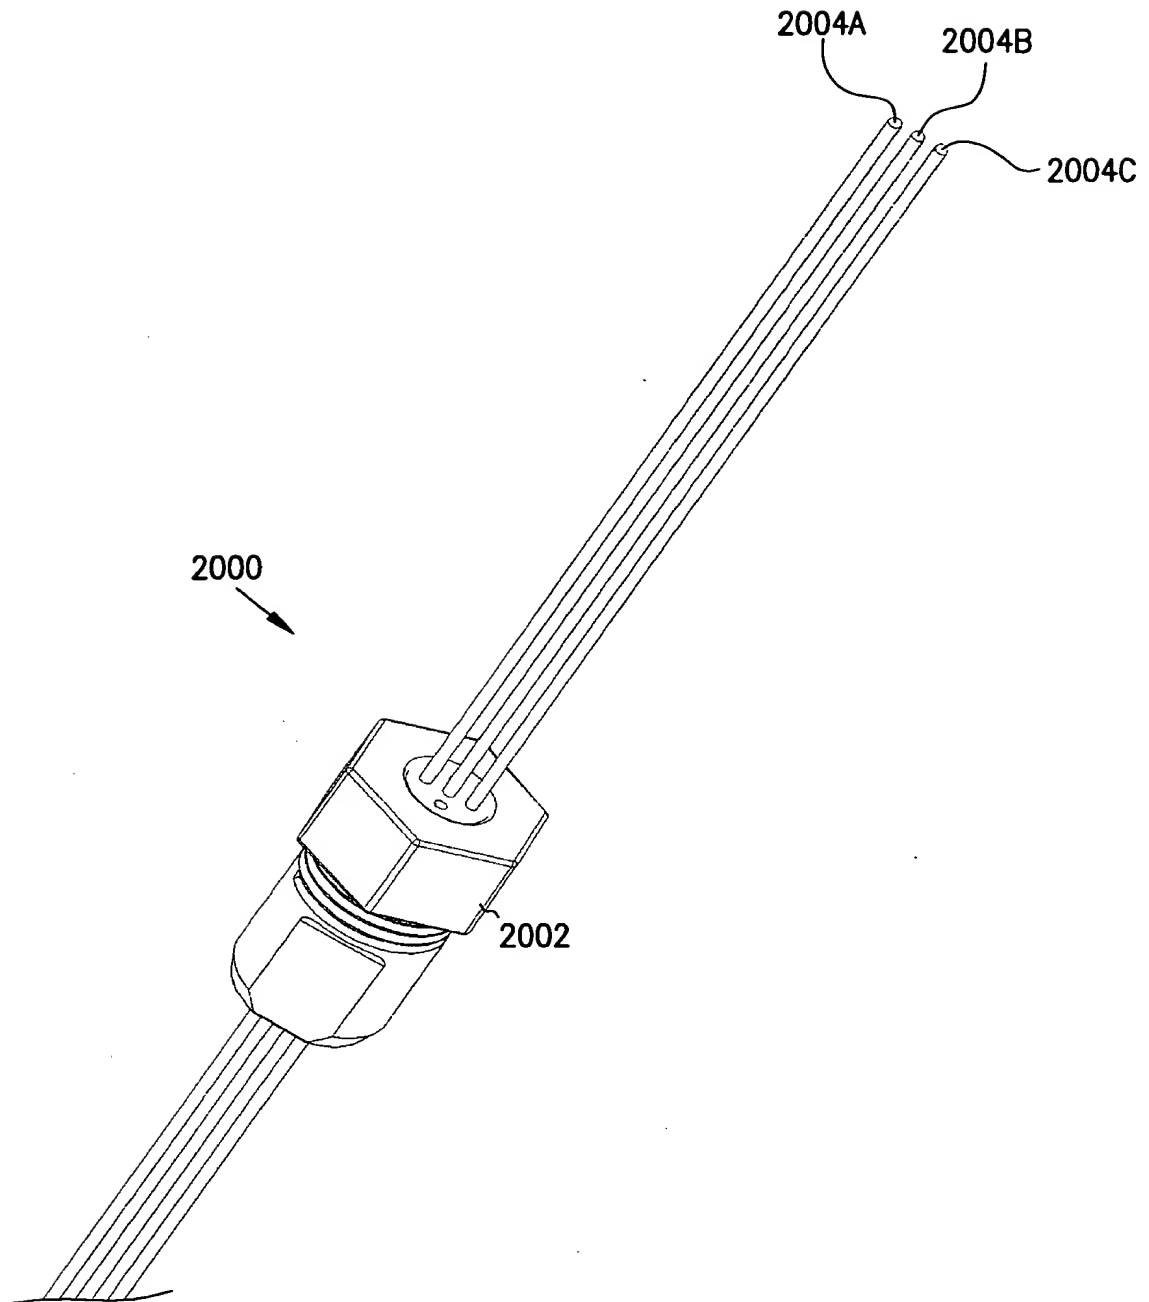


FIG. 20

09828451.082860

20/36

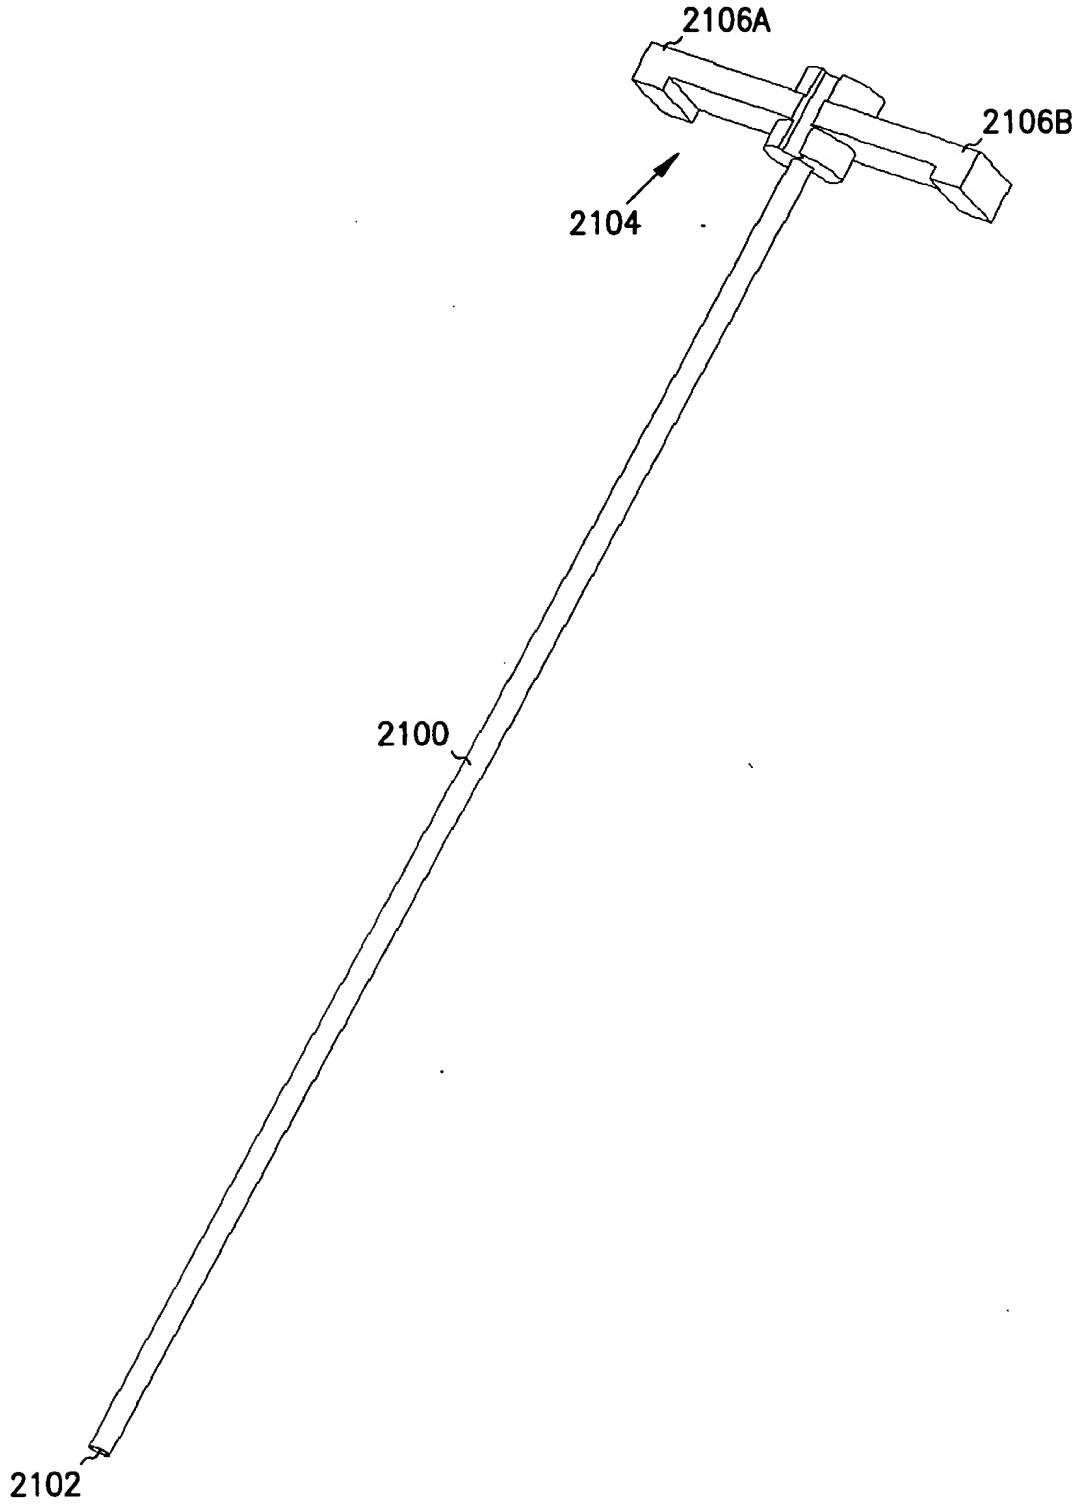


FIG. 21

09/828,451, 08/20/11

21/36

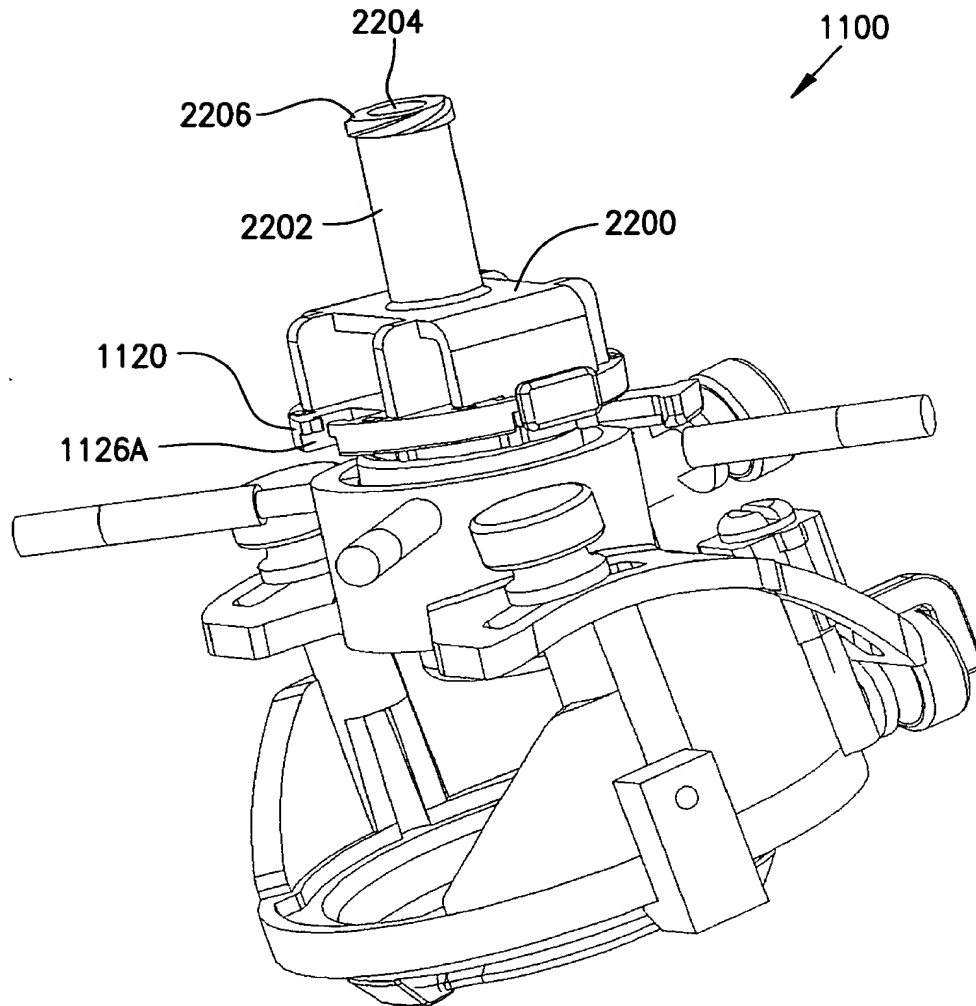


FIG. 22

09/828,451 "T-SH2260"

22/36

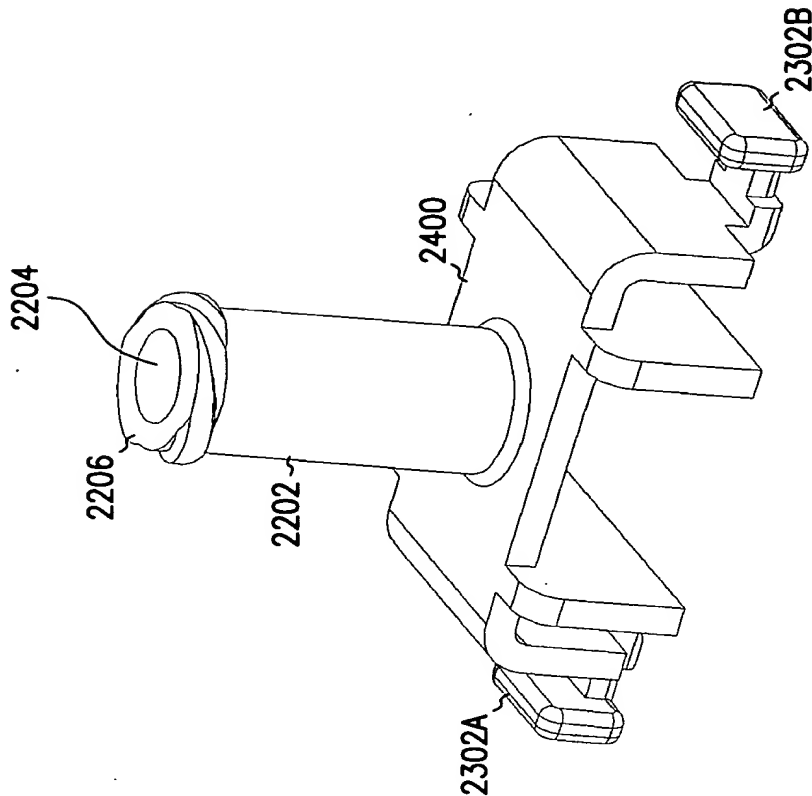


FIG. 24

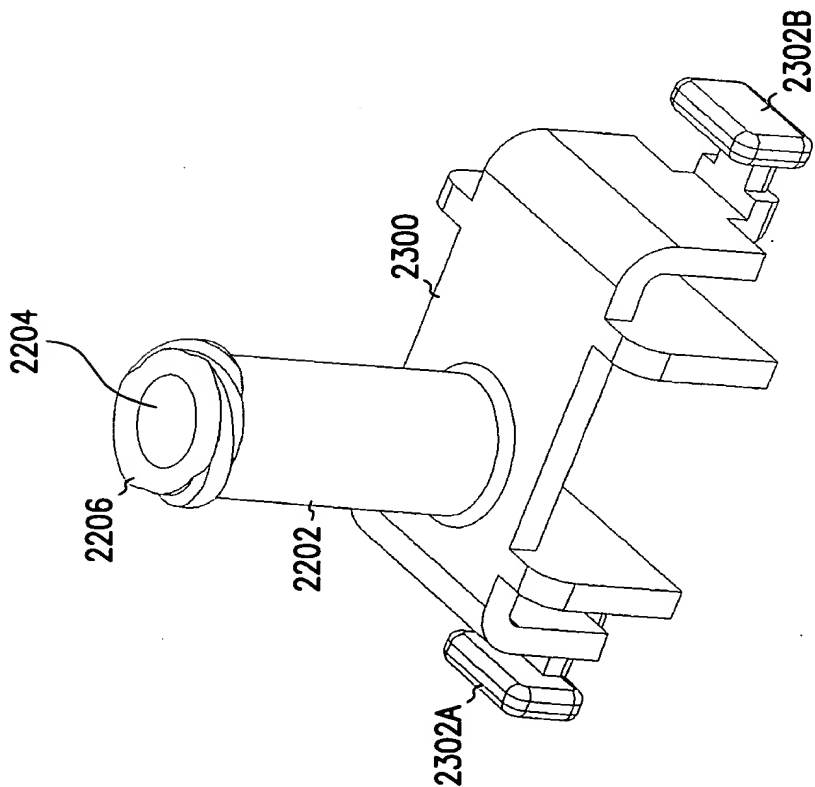


FIG. 23

TI DEEP ORGAN ACCESS DEVICE AND METHOD

23/36

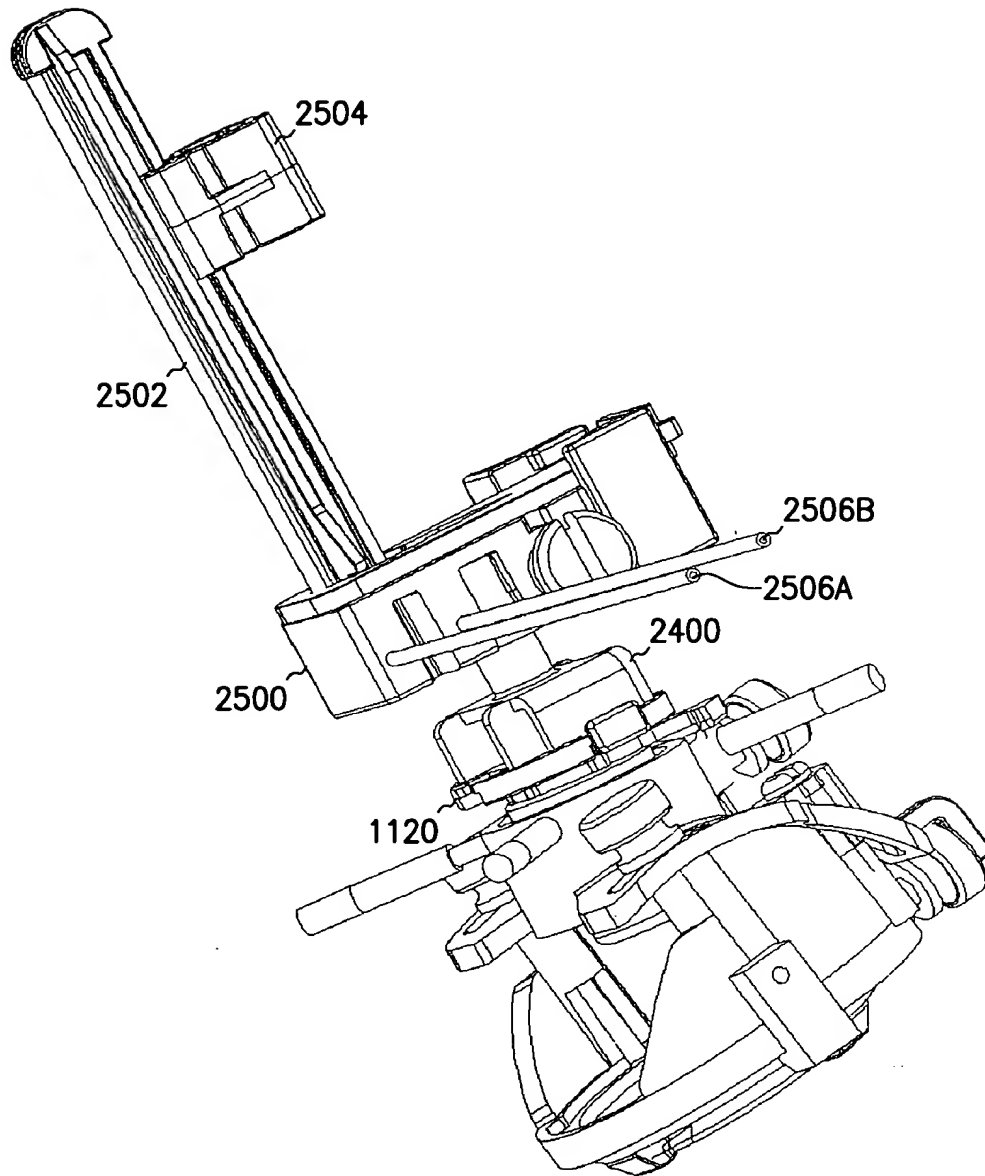


FIG. 25

09828451 082001

24/36

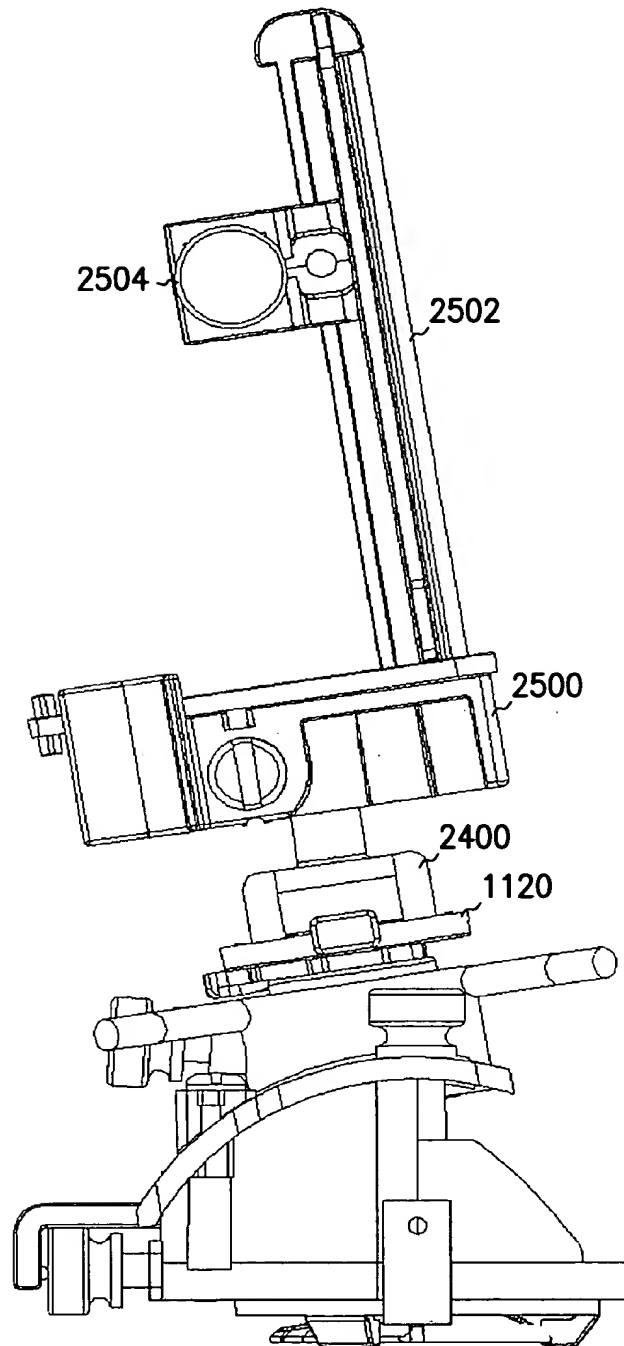


FIG. 26

09/828,451 08/2001



25/36

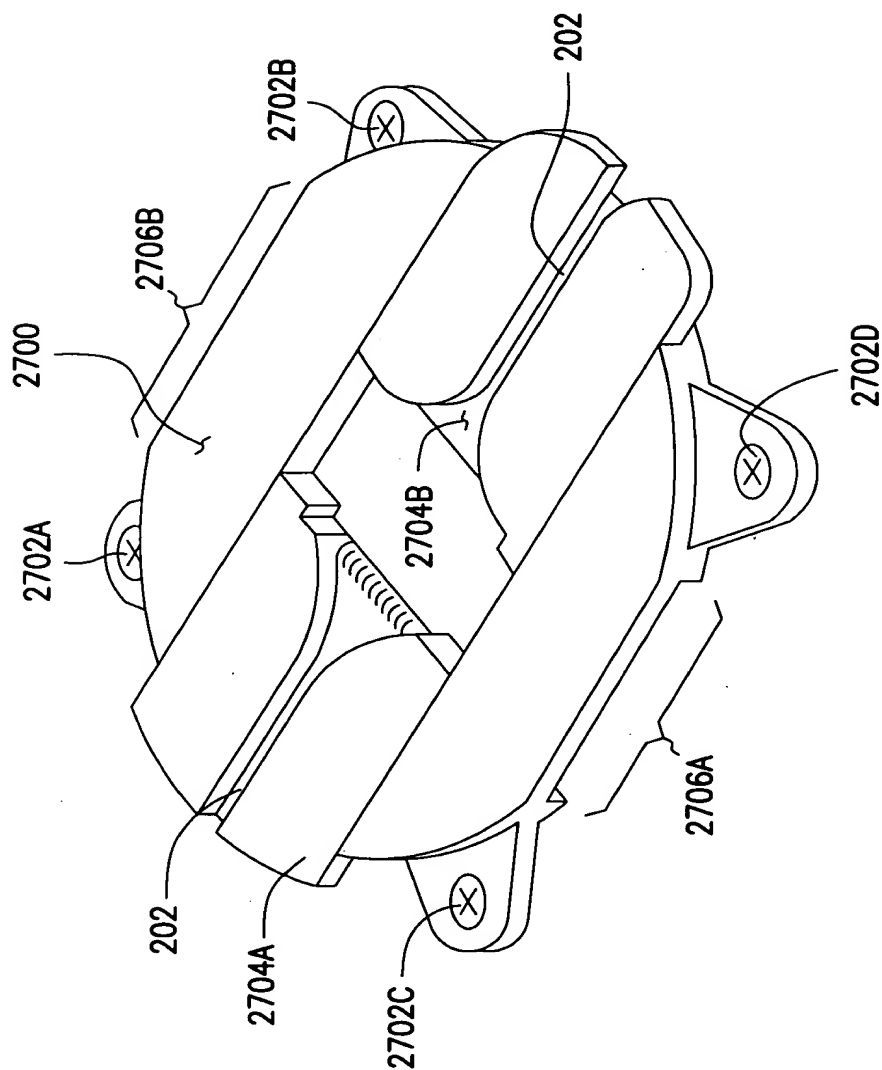


FIG. 27

TI 09/828,451

26/36

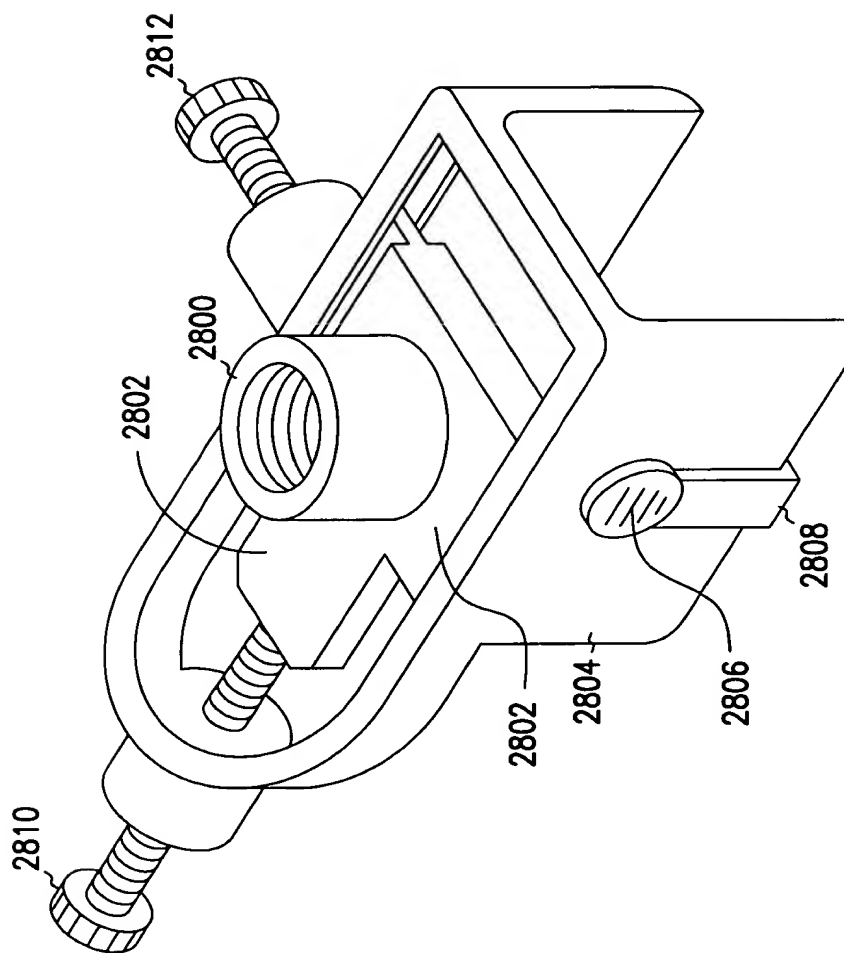


FIG. 28

FIG. 28 of 5432360

27/36

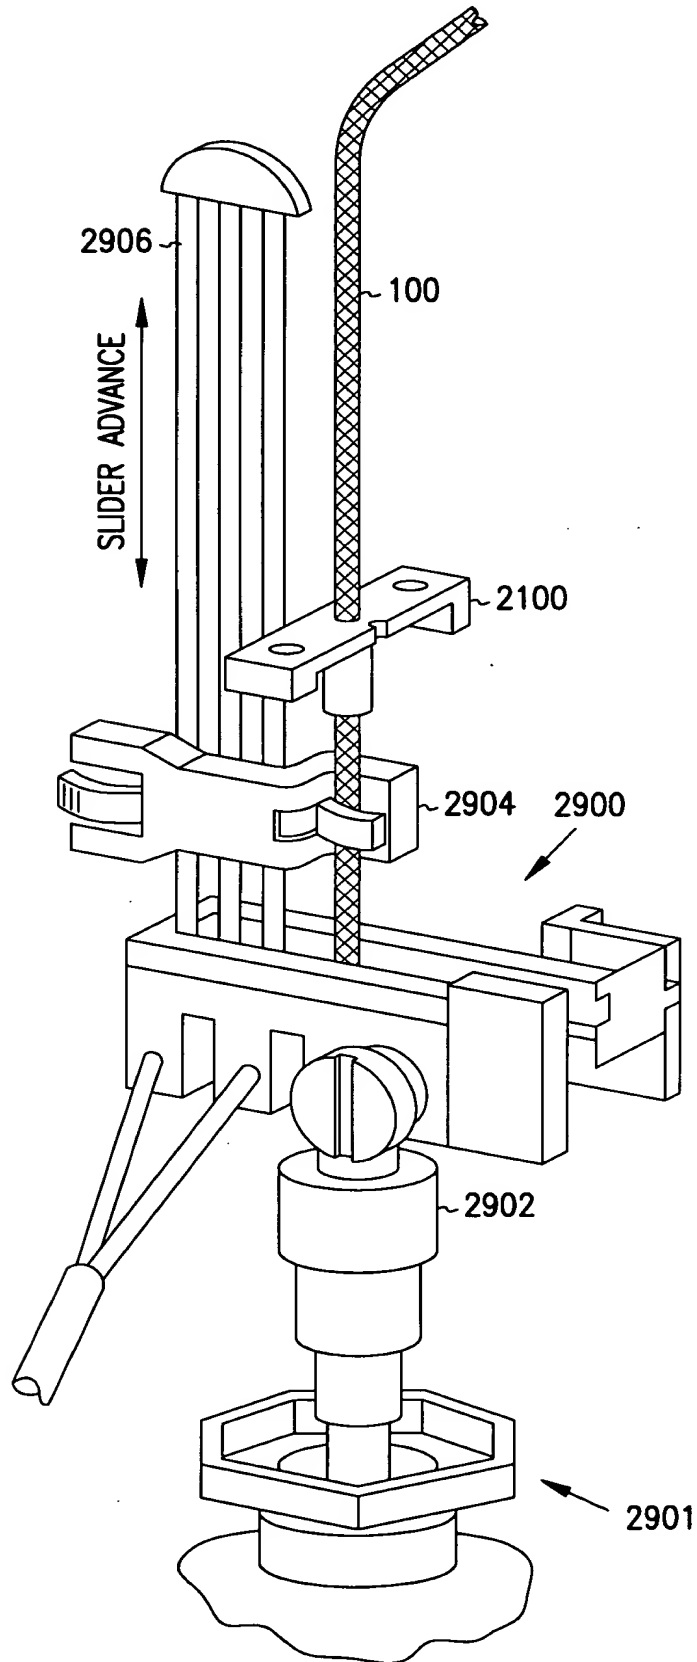


FIG. 29

09/828,451 "15482860"

28/36

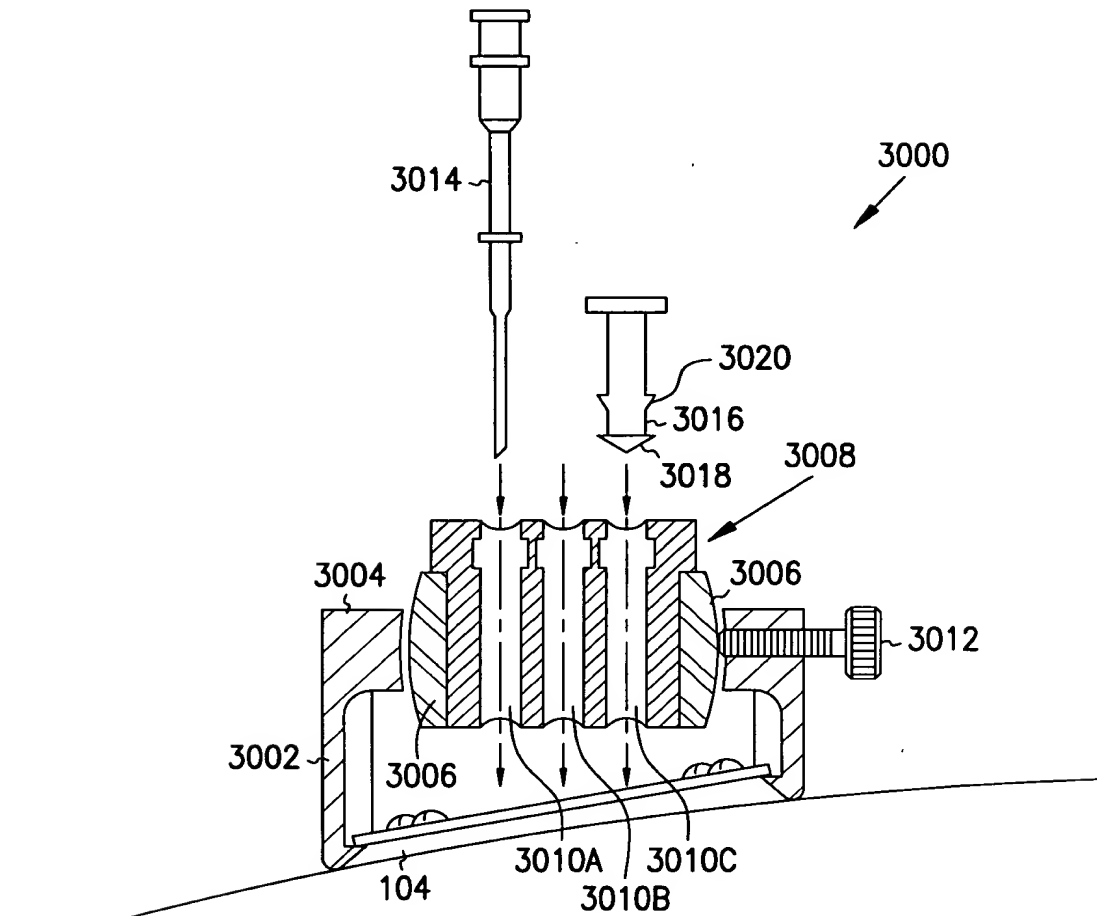


FIG. 30

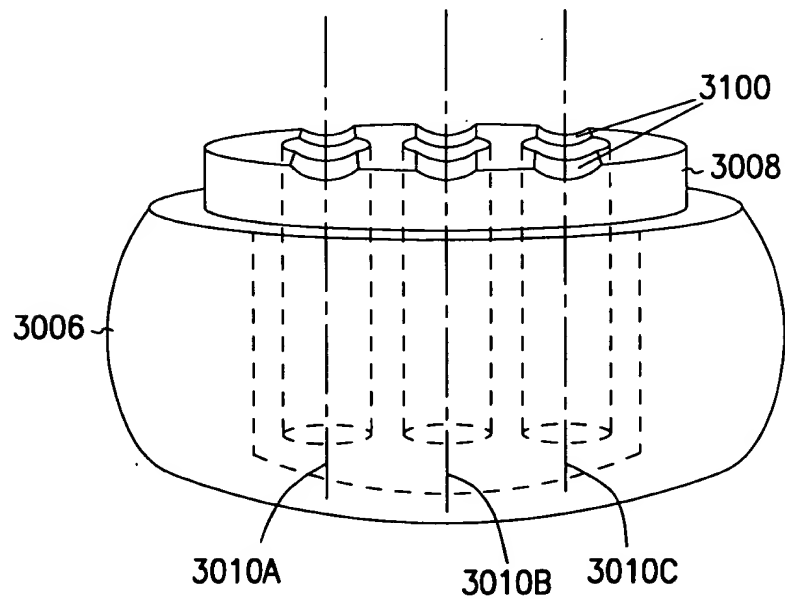


FIG. 31

29/36

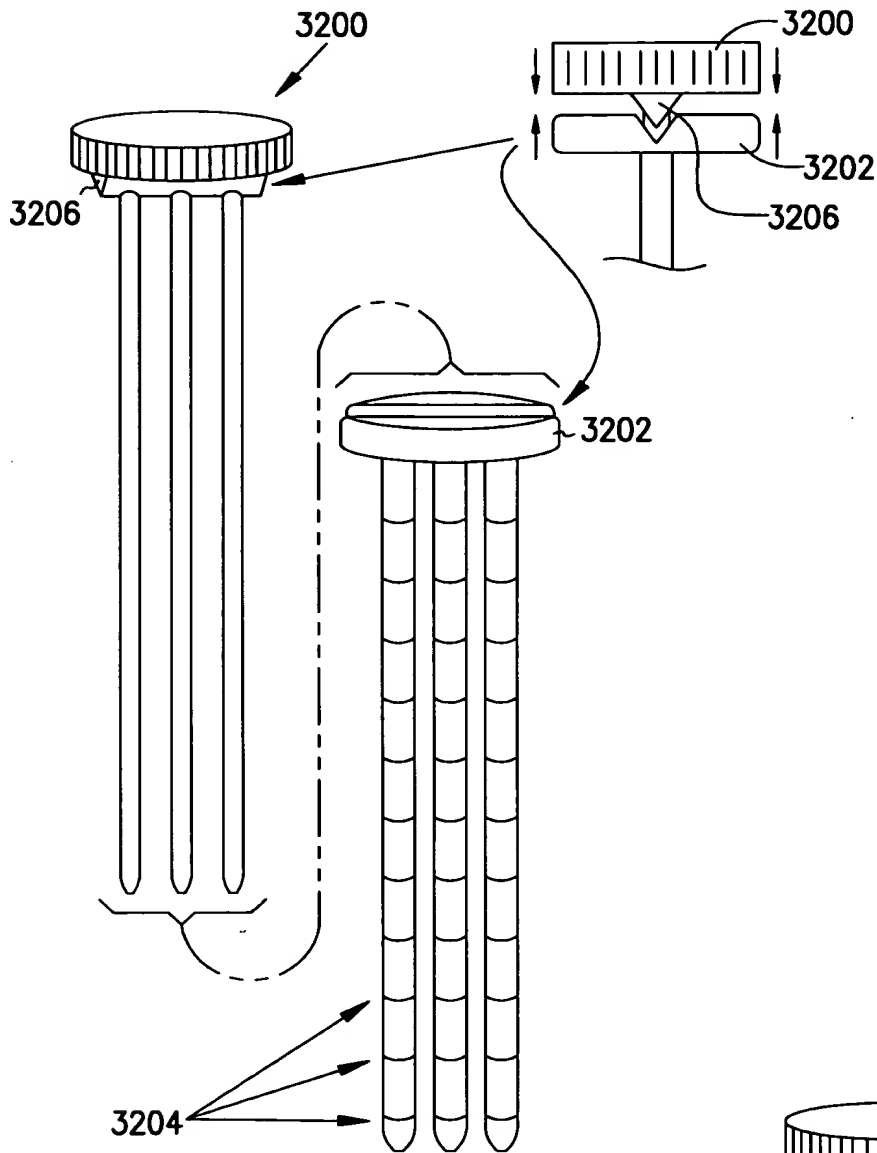


FIG. 32A






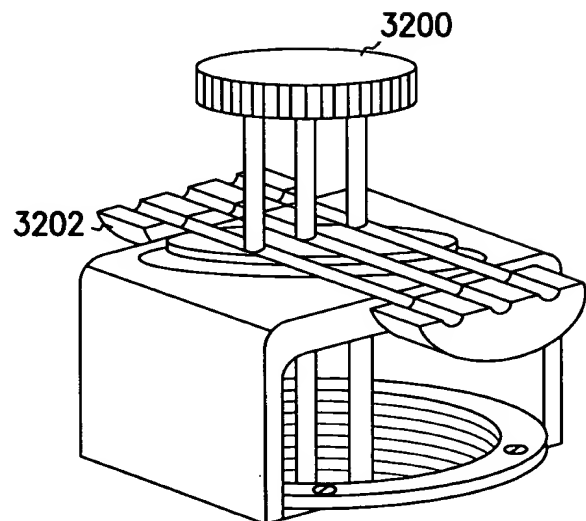


FIG. 32B

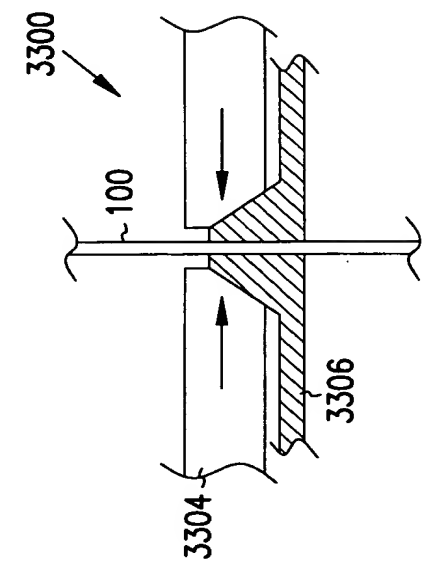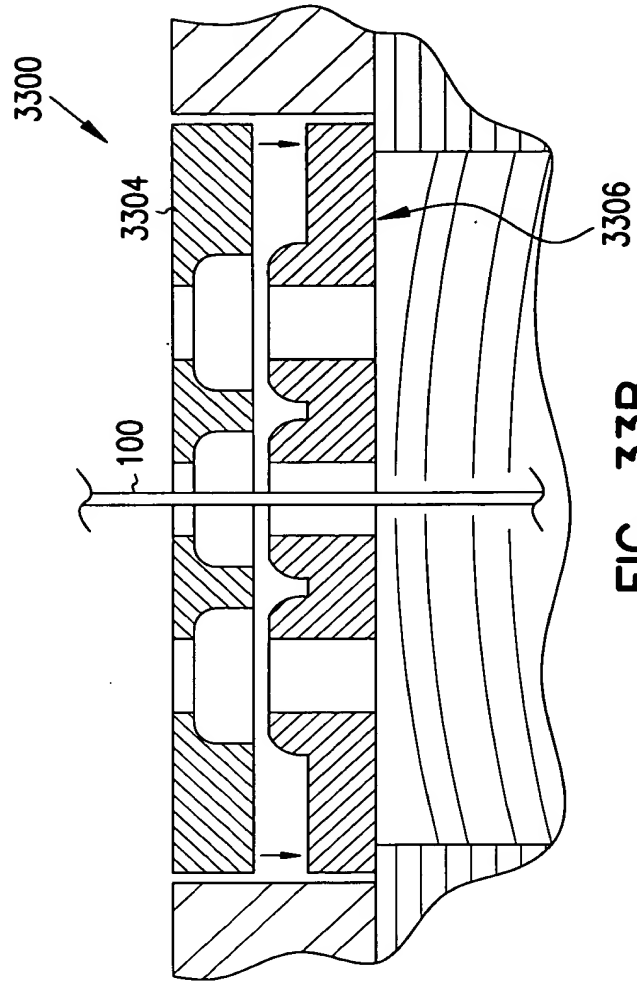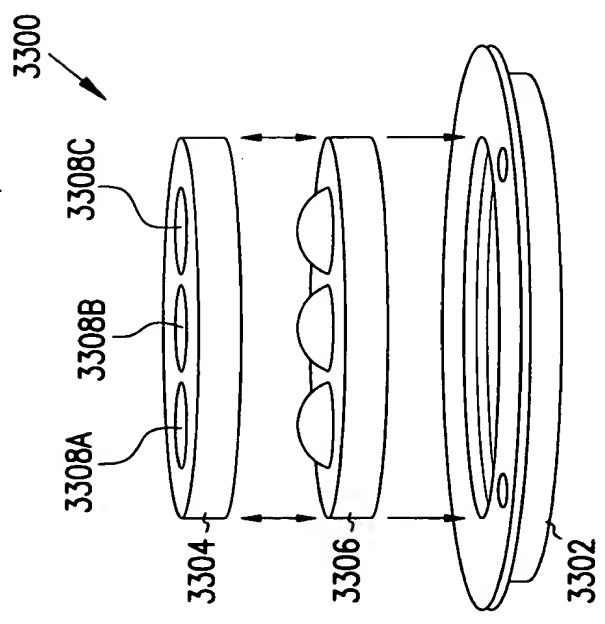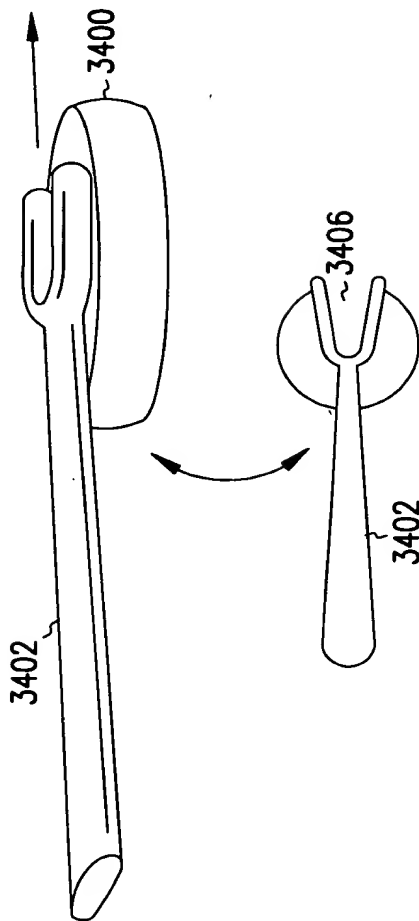

31/36

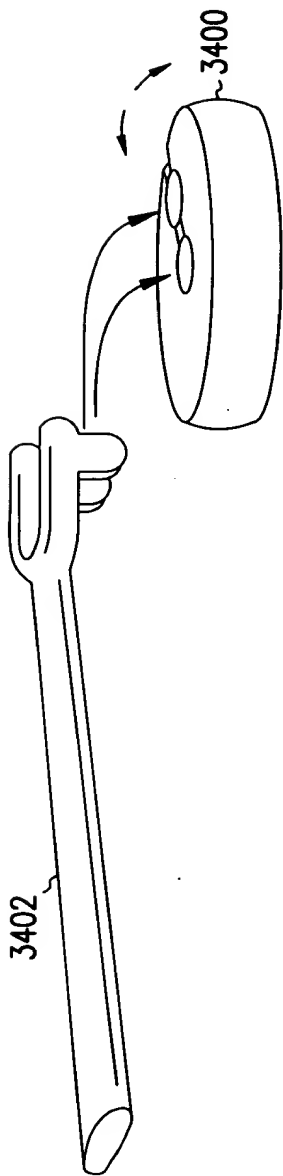

32/36

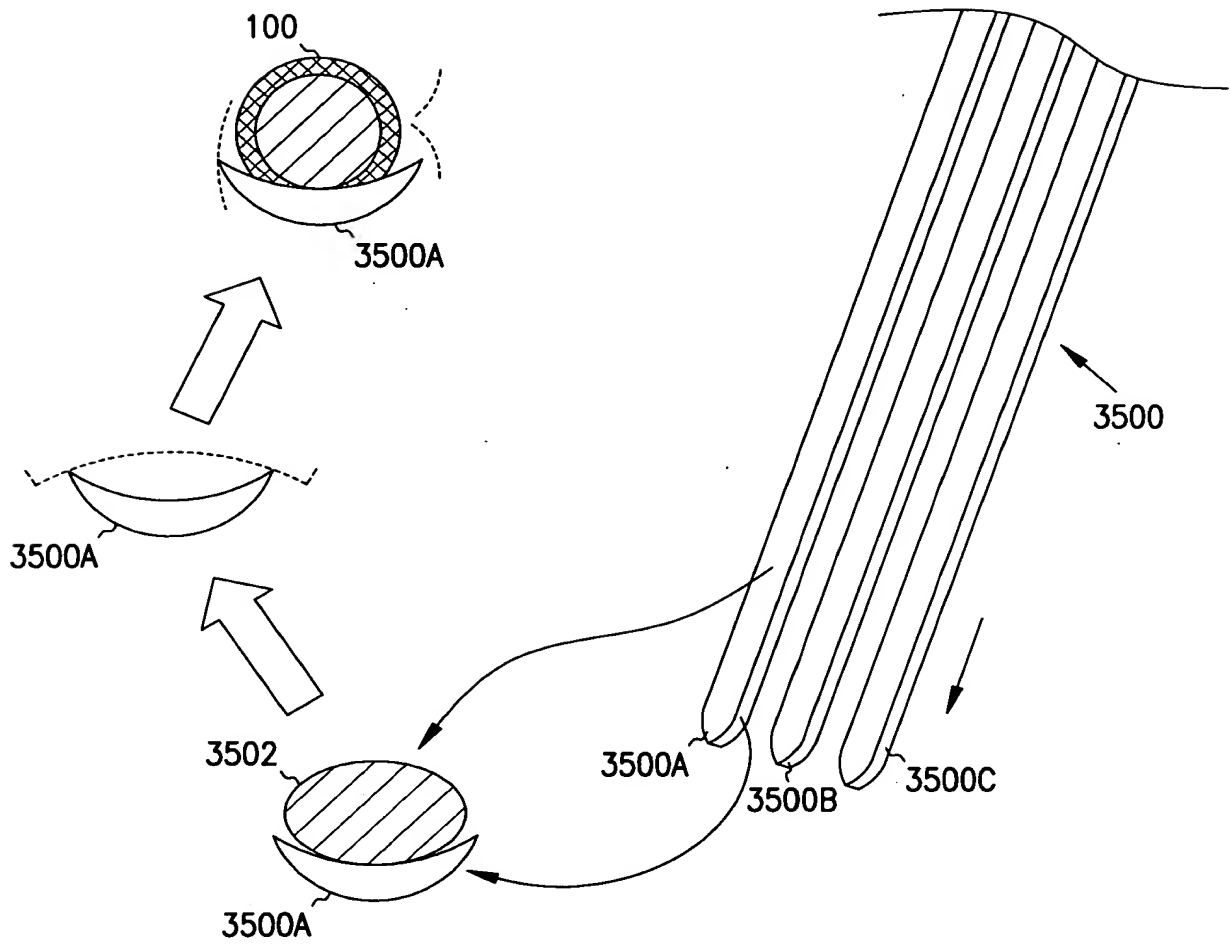


FIG. 35

09/828,451, 08/22/00



33/36

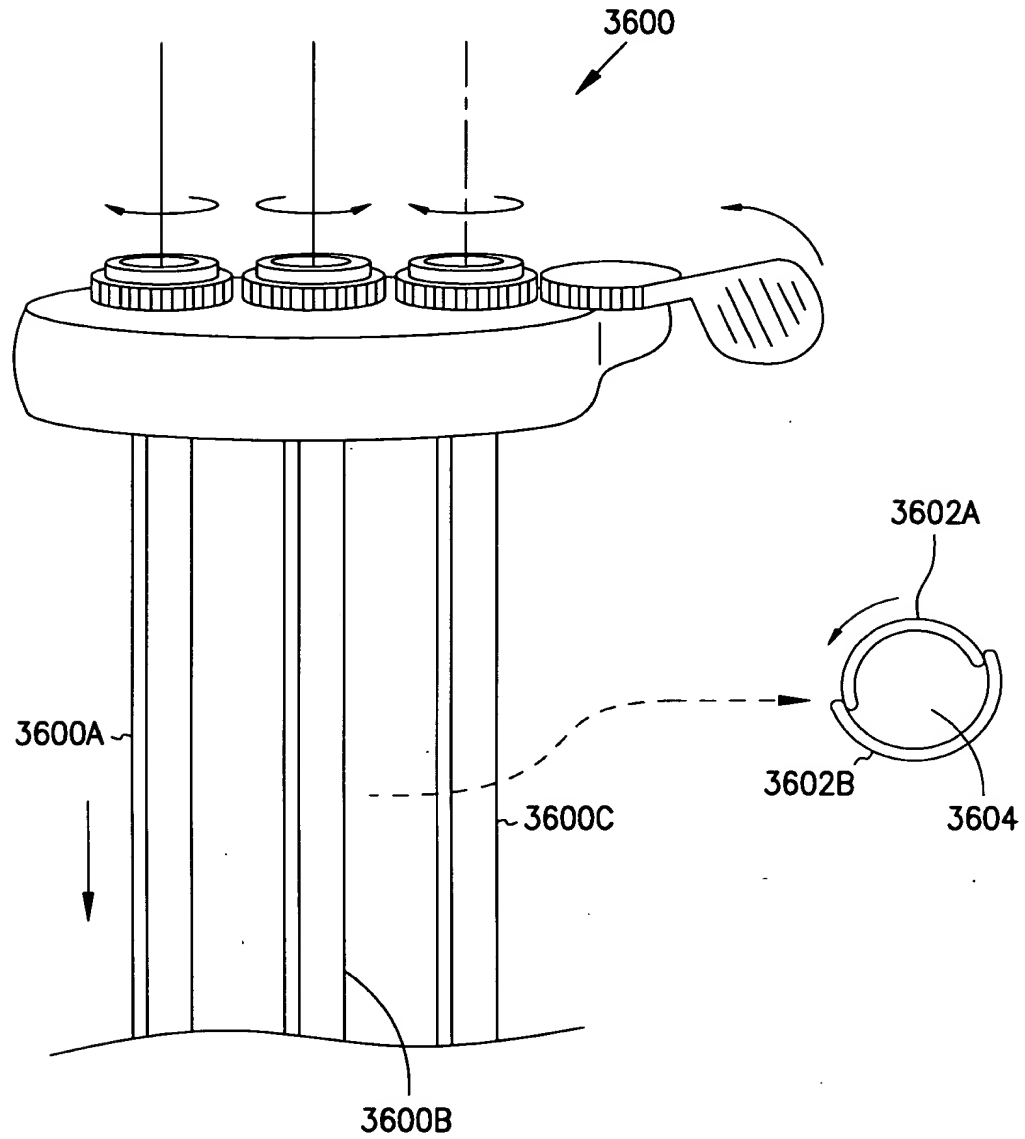


FIG. 36

34/36

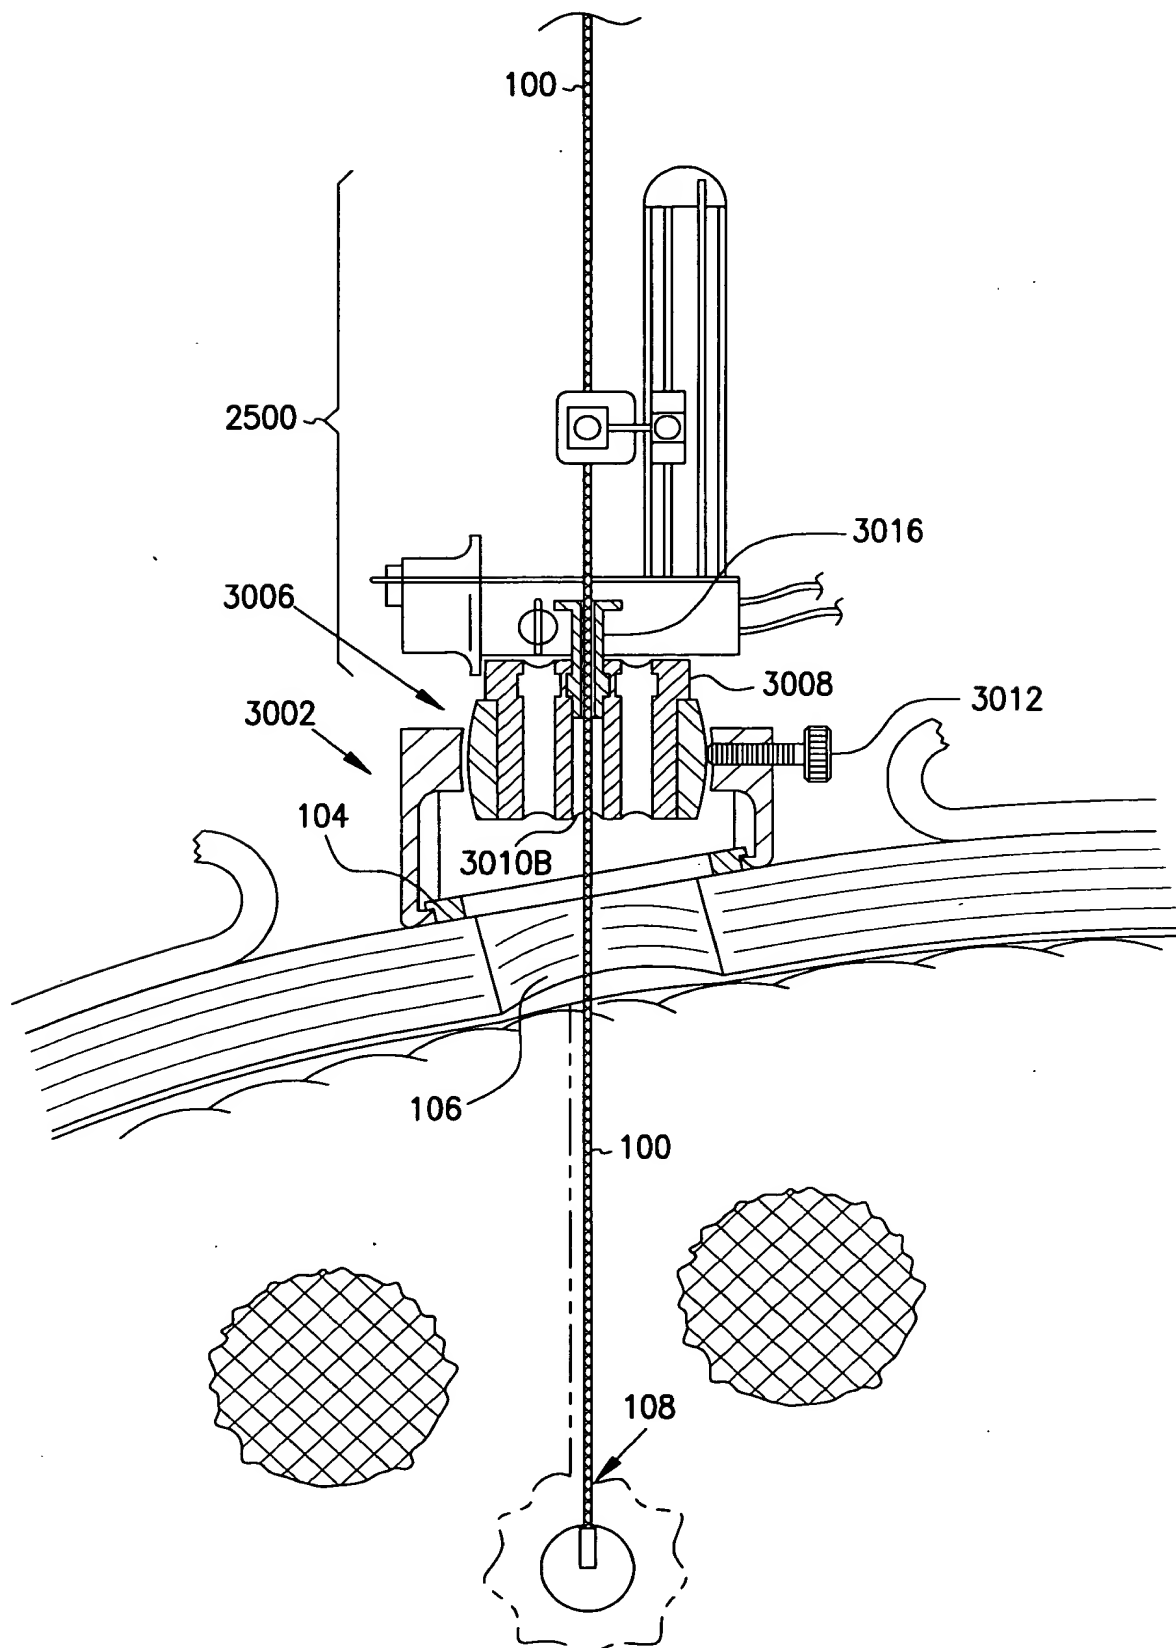


FIG. 37



36/36

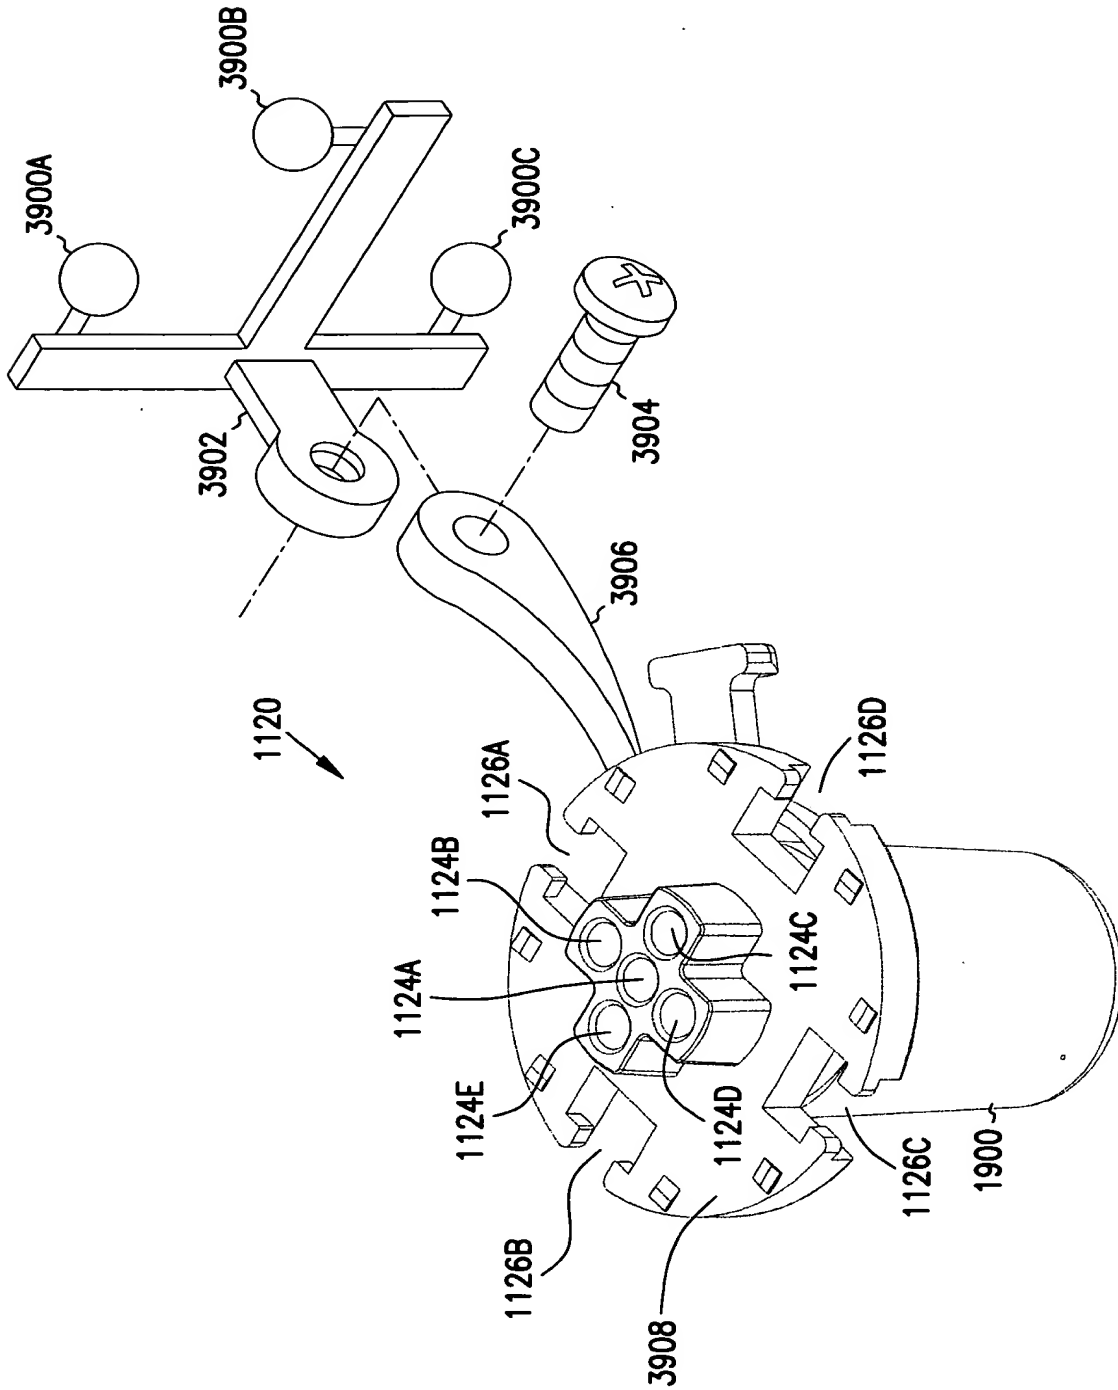


FIG. 39

FIG. 39